

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
 Data File : VV028762.D
 Acq On : 28 Oct 2022 17:19
 Operator : SY/MD
 Sample : N5232-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHAD5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028762.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	95	rBV	57548	61147	9.85%	1.265%
2	1.449	122	127	133	rBV3	10735	12436	2.00%	0.257%
3	1.565	156	163	173	rBV	64807	76203	12.28%	1.576%
4	2.105	320	331	346	rVB	118547	179556	28.93%	3.714%
5	3.896	877	888	910	rBV2	45625	151396	24.39%	3.131%
6	4.352	1010	1030	1053	rBV4	113115	389644	62.78%	8.059%
7	5.043	1227	1245	1274	rBV2	195810	516523	83.23%	10.683%
8	5.613	1410	1422	1443	rBV	221049	458924	73.95%	9.492%
9	6.066	1550	1563	1578	rBV	125524	256318	41.30%	5.301%
10	6.986	1840	1849	1868	rBV	43334	89839	14.48%	1.858%
11	7.313	1938	1951	1968	rBV	203434	369923	59.61%	7.651%
12	7.394	1970	1976	1988	rVB	12101	22263	3.59%	0.460%
13	7.622	2038	2047	2062	rBV2	23805	47327	7.63%	0.979%
14	8.092	2183	2193	2232	rBV	220474	620604	100.00%	12.836%
15	8.847	2416	2428	2458	rBV	330453	570545	91.93%	11.801%
16	9.137	2512	2518	2528	rVB5	5909	9546	1.54%	0.197%
17	10.210	2839	2852	2867	rBV	90187	149619	24.11%	3.095%
18	10.374	2896	2903	2915	rVB7	6611	11807	1.90%	0.244%
19	11.243	3161	3173	3189	rBV	309918	504166	81.24%	10.428%
20	11.616	3278	3289	3303	rBV	199555	327084	52.70%	6.765%
21	12.342	3510	3515	3525	rVB	5992	9996	1.61%	0.207%




Sum of corrected areas: 4834866

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
Data File : VV028762.D
Acq On : 28 Oct 2022 17:19
Operator : SY/MD
Sample : N5232-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

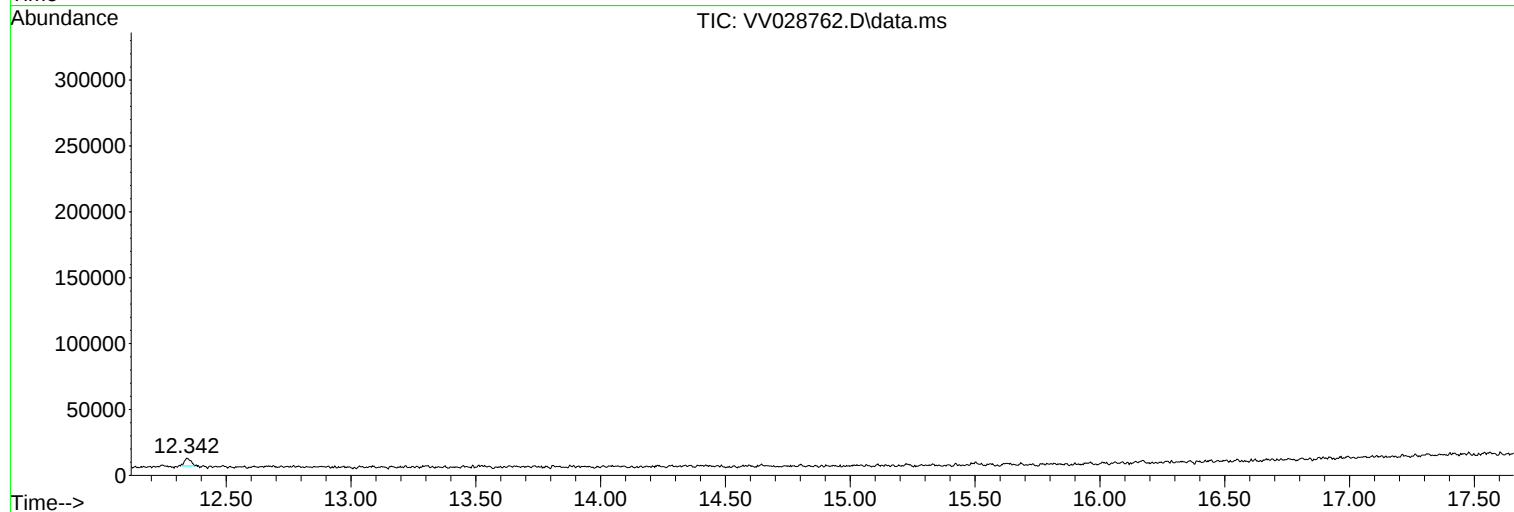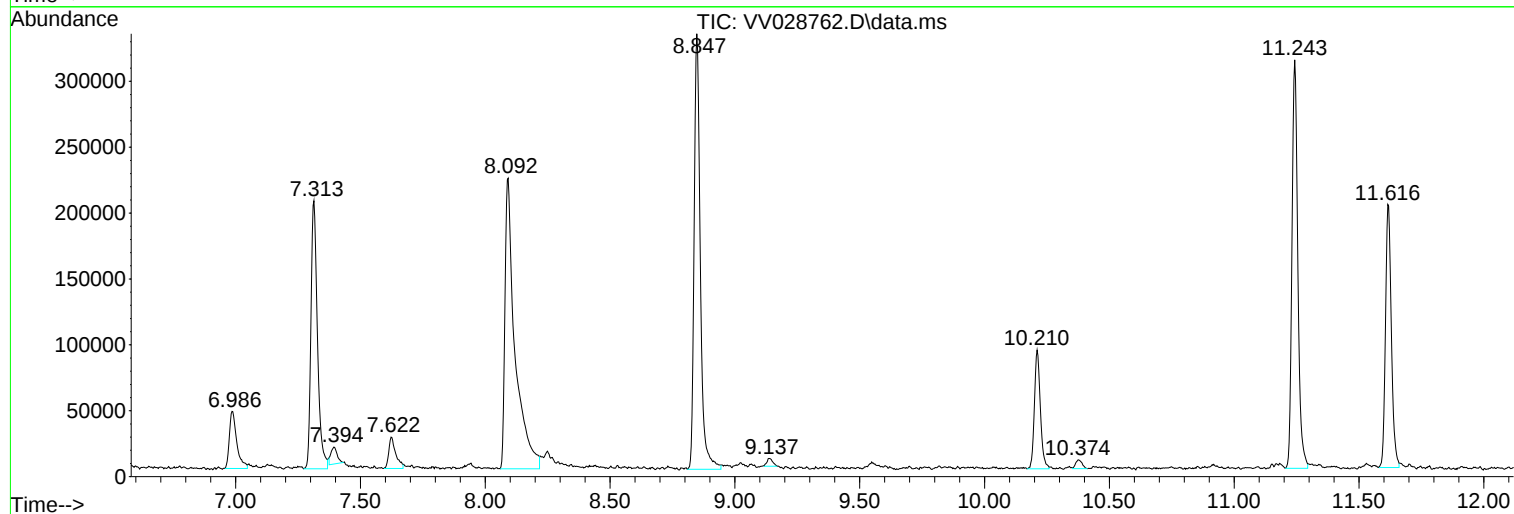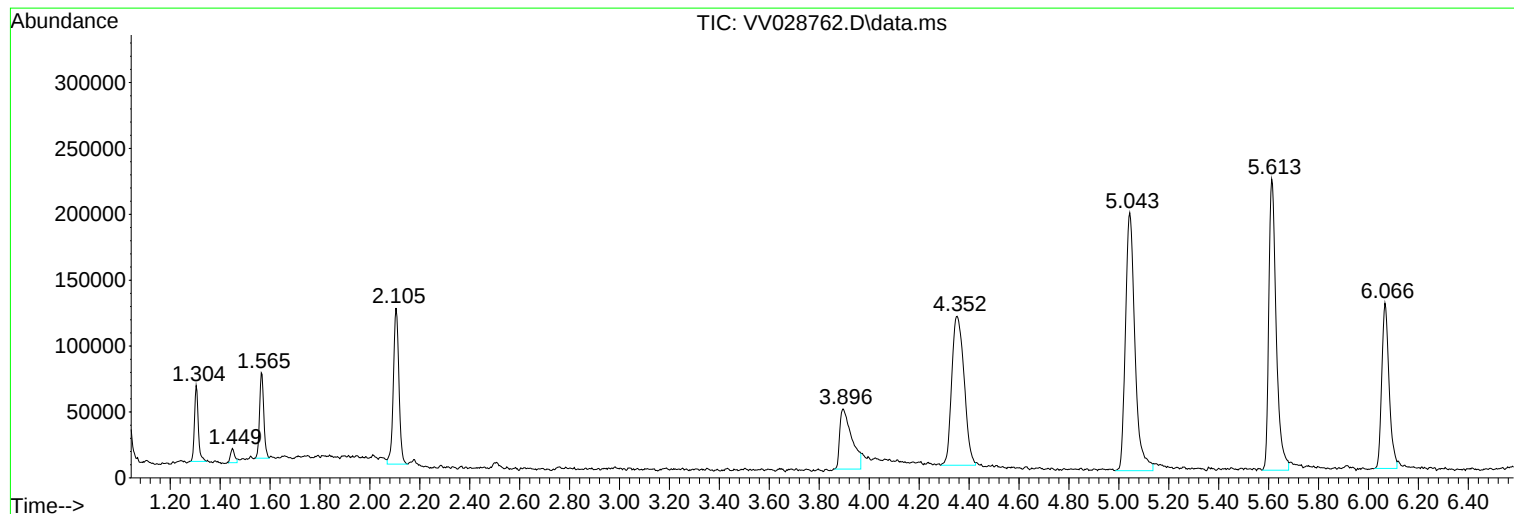

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
Data File : VV028762.D
Acq On : 28 Oct 2022 17:19
Operator : SY/MD
Sample : N5232-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
Data File : VV028762.D
Acq On : 28 Oct 2022 17:19
Operator : SY/MD
Sample : N5232-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------