

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
 Data File : VV028763.D
 Acq On : 28 Oct 2022 17:44
 Operator : SY/MD
 Sample : N5232-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHAD6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028763.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	92	rBV	57431	58733	9.35%	1.228%
2	1.564	156	163	176	rBV	66490	78028	12.42%	1.631%
3	2.105	322	331	347	rVB	117952	175213	27.89%	3.662%
4	3.896	880	888	915	rBV2	39506	144091	22.94%	3.011%
5	4.349	1013	1029	1058	rVB3	113157	392533	62.48%	8.204%
6	5.043	1230	1245	1268	rBV2	193395	495810	78.92%	10.362%
7	5.613	1411	1422	1447	rBV	213714	453562	72.20%	9.479%
8	6.066	1551	1563	1588	rBV2	126592	266157	42.37%	5.563%
9	6.985	1838	1849	1869	rBV2	44368	87287	13.89%	1.824%
10	7.313	1940	1951	1970	rBV	201997	368317	58.63%	7.698%
11	7.394	1970	1976	1986	rVB2	12069	21333	3.40%	0.446%
12	7.622	2040	2047	2065	rBV	23238	45047	7.17%	0.941%
13	8.092	2182	2193	2231	rBV	219901	628222	100.00%	13.130%
14	8.847	2413	2428	2450	rBV	319230	549705	87.50%	11.489%
15	9.143	2512	2520	2529	rVB8	8003	13328	2.12%	0.279%
16	9.545	2635	2645	2648	rBV8	6236	8332	1.33%	0.174%
17	10.210	2840	2852	2865	rBV	89101	150502	23.96%	3.145%
18	10.378	2894	2904	2911	rBV4	7625	12948	2.06%	0.271%
19	11.243	3161	3173	3193	rBV	303637	492425	78.38%	10.292%
20	11.619	3278	3290	3308	rBV	195236	327183	52.08%	6.838%
21	12.349	3507	3517	3528	rBV	7963	15978	2.54%	0.334%




Sum of corrected areas: 4784734

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
Data File : VV028763.D
Acq On : 28 Oct 2022 17:44
Operator : SY/MD
Sample : N5232-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

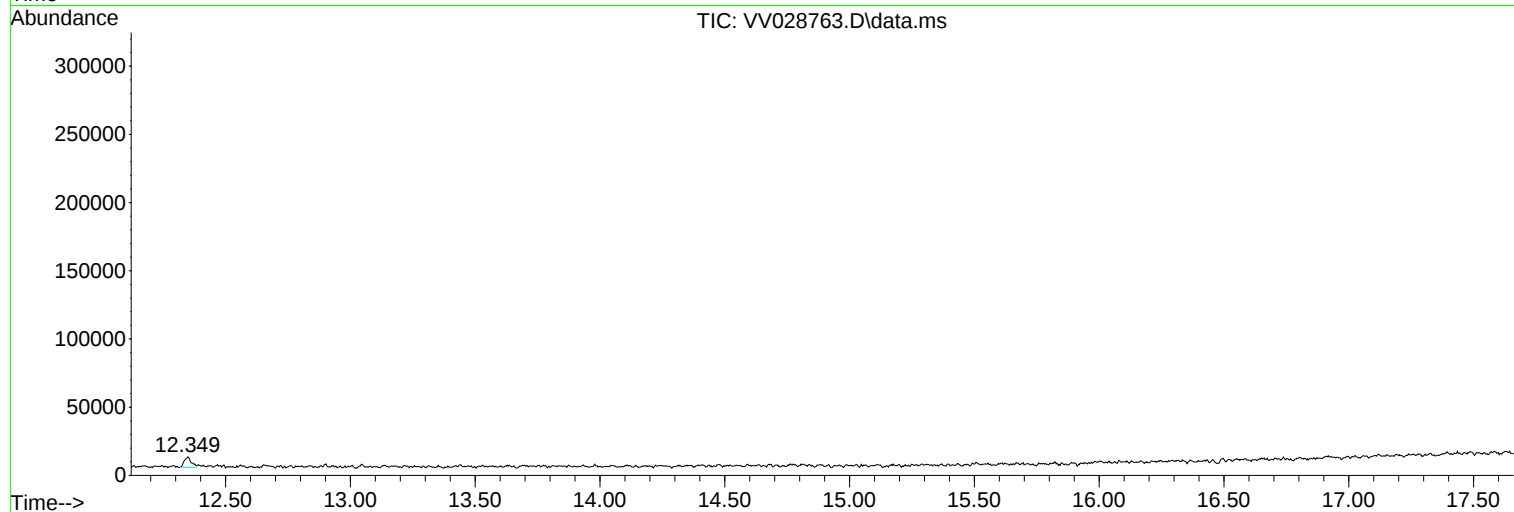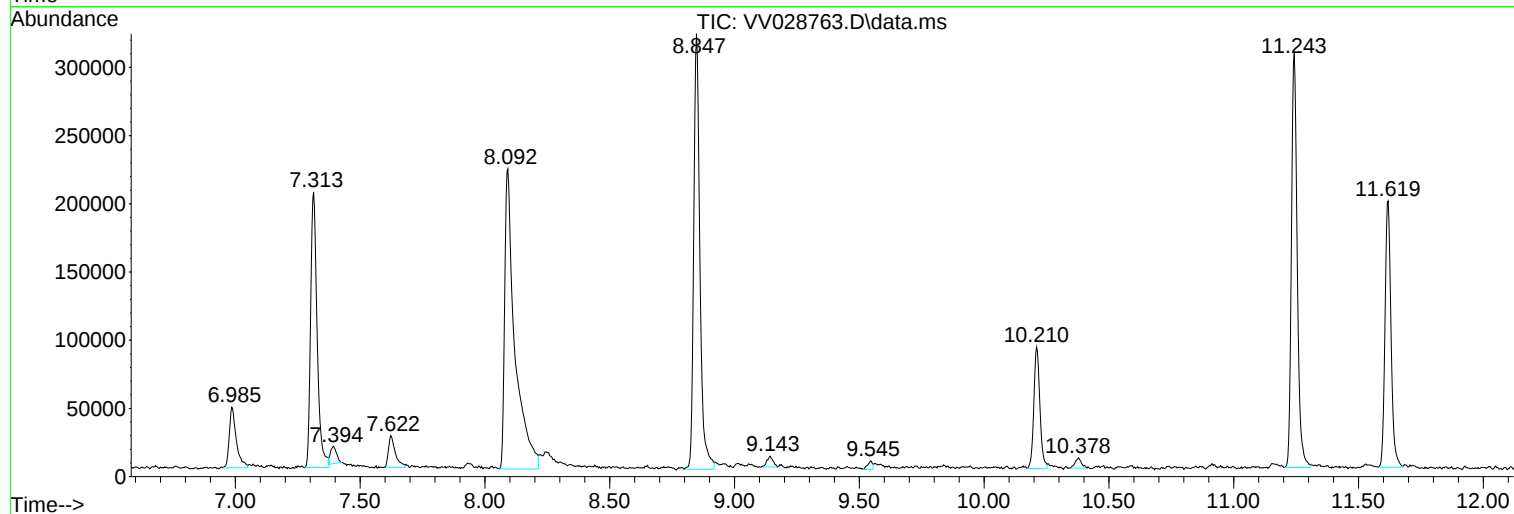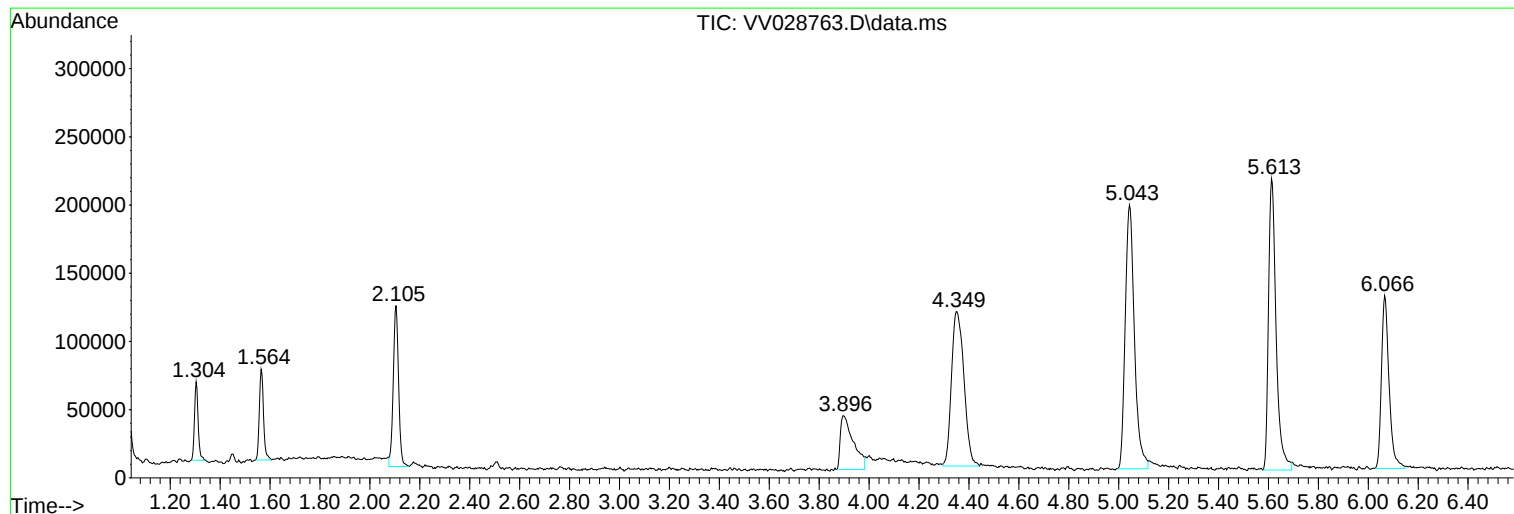

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
Data File : VV028763.D
Acq On : 28 Oct 2022 17:44
Operator : SY/MD
Sample : N5232-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
Data File : VV028763.D
Acq On : 28 Oct 2022 17:44
Operator : SY/MD
Sample : N5232-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------