

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
 Data File : VV028764.D
 Acq On : 28 Oct 2022 18:08
 Operator : SY/MD
 Sample : N5232-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028764.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rBV	104416	108795	19.08%	2.270%
2	1.445	121	126	134	rBV	16816	19179	3.36%	0.400%
3	1.564	155	163	173	rBV	88519	101295	17.76%	2.114%
4	2.101	321	330	347	rVB	181591	267890	46.98%	5.589%
5	2.500	447	454	460	rBV7	4867	6447	1.13%	0.135%
6	3.908	882	892	916	rBV2	30466	116105	20.36%	2.423%
7	4.342	1009	1027	1051	rBV2	95453	244372	42.86%	5.099%
8	5.043	1231	1245	1266	rBV2	232169	570218	100.00%	11.897%
9	5.612	1410	1422	1444	rBV	211325	436438	76.54%	9.106%
10	6.066	1549	1563	1583	rBV	136853	288523	50.60%	6.020%
11	6.985	1839	1849	1871	rBV2	48303	101705	17.84%	2.122%
12	7.310	1939	1950	1971	rBV	256531	465825	81.69%	9.719%
13	7.625	2038	2048	2063	rBV	25847	51729	9.07%	1.079%
14	8.091	2182	2193	2229	rBV	181992	504677	88.51%	10.530%
15	8.847	2417	2428	2452	rBV	320137	538267	94.40%	11.231%
16	10.210	2842	2852	2865	rBV	79084	127730	22.40%	2.665%
17	10.374	2895	2903	2913	rVB9	6878	11293	1.98%	0.236%
18	11.242	3163	3173	3193	rBV	300312	477688	83.77%	9.967%
19	11.615	3278	3289	3309	rBV	211027	354579	62.18%	7.398%




Sum of corrected areas: 4792755

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
Data File : VV028764.D
Acq On : 28 Oct 2022 18:08
Operator : SY/MD
Sample : N5232-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

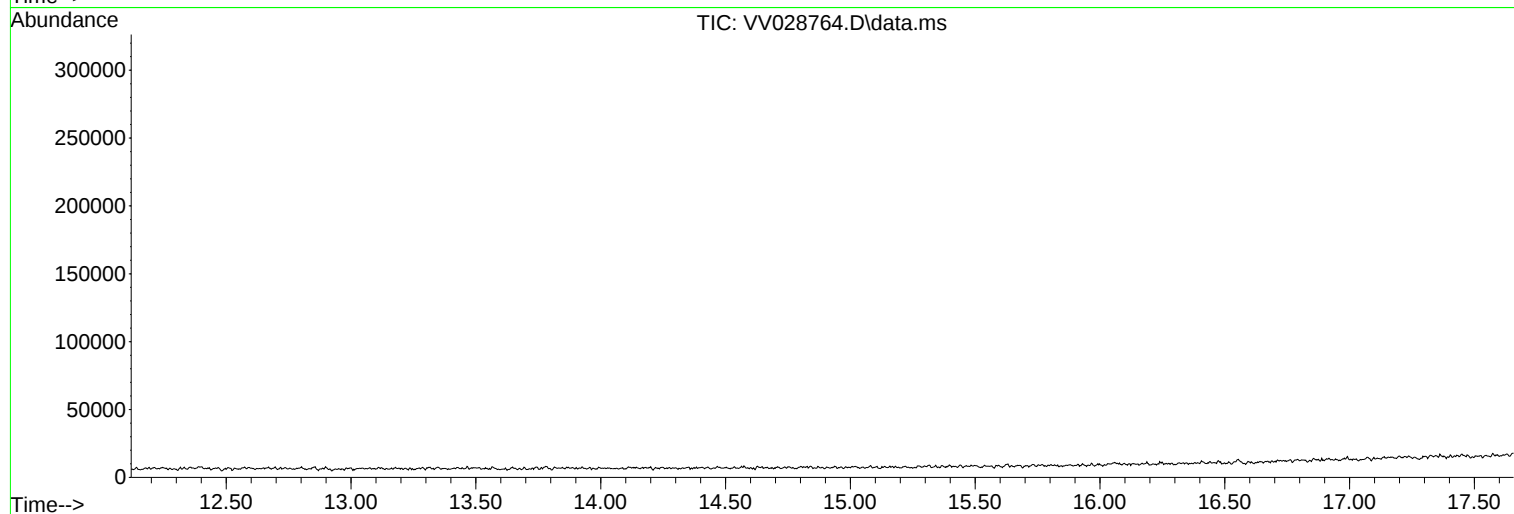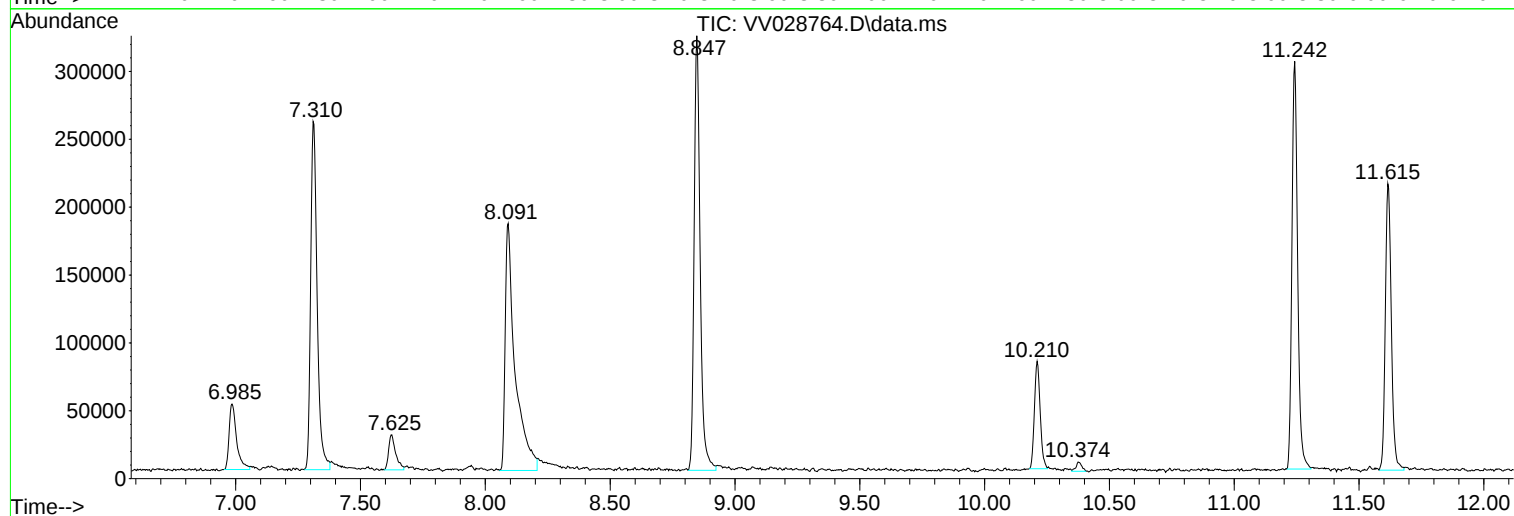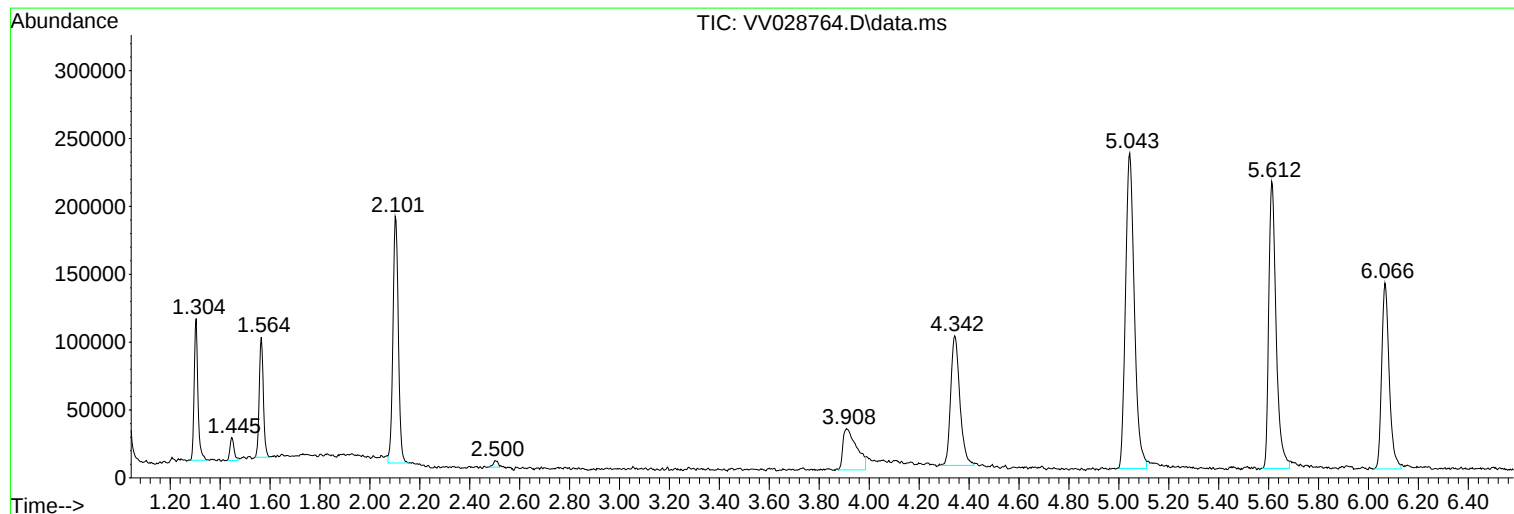

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
Data File : VV028764.D
Acq On : 28 Oct 2022 18:08
Operator : SY/MD
Sample : N5232-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
Data File : VV028764.D
Acq On : 28 Oct 2022 18:08
Operator : SY/MD
Sample : N5232-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc