
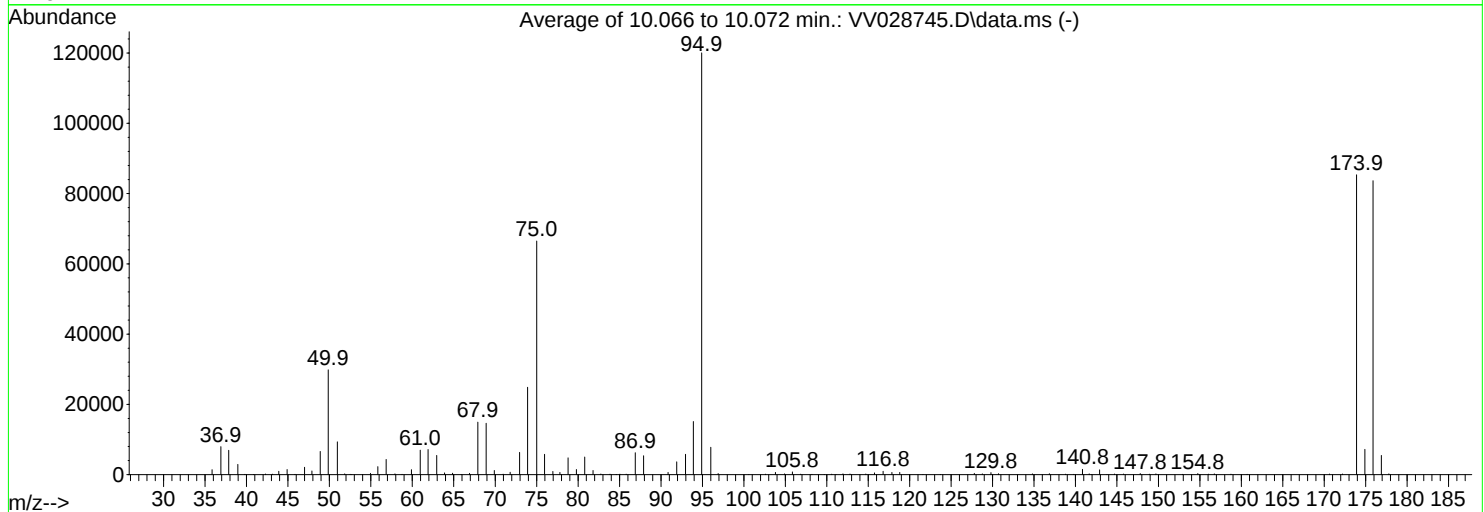


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
 Data File : VV028745.D
 Acq On : 28 Oct 2022 09:03
 Operator : SY/MD
 Sample : BFB393
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB393

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Oct 28 21:50:06 2022

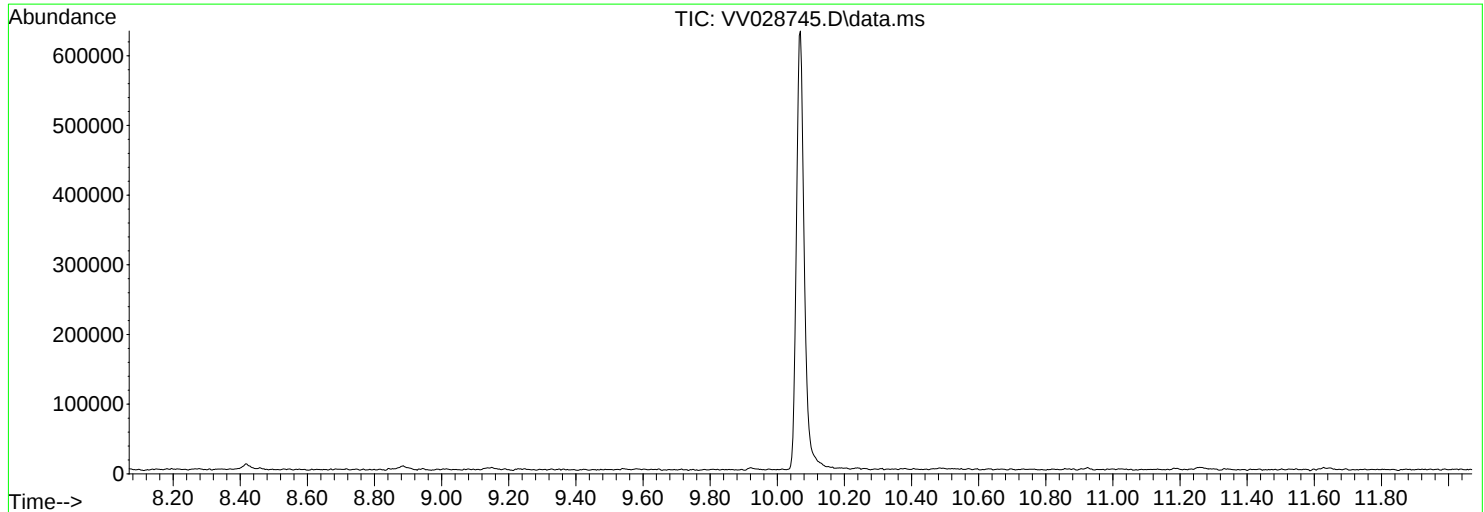

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.9	29852	PASS
75	95	30	80	55.4	66499	PASS
95	95	100	100	100.0	120056	PASS
96	95	5	9	6.5	7768	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.1	85325	PASS
175	174	5	9	8.5	7210	PASS
176	174	95	105	98.0	83661	PASS
177	176	5	10	6.5	5447	PASS

m/z	Abundance
35.30	154.0
35.90	199.0
36.60	164.0
37.10	162.0
37.70	185.0
38.40	173.0
39.80	1114.0
41.00	137.0
42.00	186.0
42.70	134.0
43.90	623.0
45.90	103.0
46.40	116.0
47.60	107.0
47.90	116.0
48.90	112.0
49.80	121.0
51.80	122.0
53.50	123.0
55.00	115.0
55.80	168.0
56.80	145.0
59.50	111.0
60.50	135.0
65.30	113.0
71.80	118.0
73.00	135.0
74.80	136.0
76.10	119.0
84.10	101.0
85.30	136.0
101.40	120.0
102.30	107.0
142.90	103.0
176.50	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB393

m/z	Abundance
35.90	1660.0
36.90	8633.0
37.90	7293.0
39.00	3154.0
39.80	1139.0
40.80	199.0
41.80	172.0
42.30	164.0
43.20	186.0
43.90	1607.0
44.90	1467.0
45.80	223.0
46.20	170.0
47.00	2249.0
47.90	1197.0
48.90	6966.0
49.90	31136.0
51.00	9761.0
51.90	352.0
52.50	165.0
53.60	112.0
55.00	567.0
55.90	2560.0
56.90	4457.0
57.90	183.0
58.70	106.0
59.90	1458.0
61.00	7132.0
61.90	7258.0
62.90	5566.0
63.90	517.0
64.80	375.0
66.90	400.0
67.90	15398.0
68.90	15074.0
69.90	1255.0
70.90	135.0
71.90	929.0
73.00	6535.0
73.90	25344.0
75.00	69072.0
76.00	6048.0
77.00	998.0
77.80	667.0
78.80	4990.0
79.80	1568.0
80.80	5285.0
81.80	1223.0
82.70	159.0
83.80	105.0
85.00	135.0
85.80	215.0
86.90	6454.0
87.90	5528.0
90.80	649.0
91.90	3620.0
92.90	5854.0
93.90	15653.0
94.90	123112.0
96.00	7977.0
96.90	315.0
102.60	127.0
103.80	630.0
104.90	238.0
105.80	706.0
106.90	170.0
109.70	127.0
110.60	128.0
111.10	136.0
111.90	210.0
112.70	215.0
114.80	199.0
115.70	555.0
116.80	1000.0
117.90	675.0
118.80	713.0
127.80	375.0
128.70	235.0
129.80	652.0
130.70	250.0
134.80	290.0
136.90	268.0
138.80	114.0
139.90	116.0
140.80	1637.0
141.70	267.0
142.90	1509.0
144.70	178.0
145.80	194.0
147.80	327.0
148.90	139.0
149.70	235.0

Instrument :
MSVOA_V
ClientSampleId :
BFB393

154.70	309.0
156.10	138.0
156.70	224.0
158.70	168.0
160.70	137.0
170.70	141.0
172.20	491.0
173.90	84680.0
174.90	7214.0
175.90	84152.0
176.90	5438.0
177.80	264.0

Instrument :
MSVOA_V
ClientSampleId :
BFB393

m/z	Abundance
35.90	1651.0
36.90	8414.0
37.90	7195.0
39.00	2968.0
39.80	1209.0
40.80	187.0
41.90	154.0
42.30	172.0
42.80	183.0
43.10	176.0
43.90	1596.0
44.90	1499.0
45.80	207.0
47.00	2228.0
47.90	1168.0
48.90	7005.0
49.90	31120.0
50.90	9588.0
51.90	356.0
52.50	142.0
53.60	107.0
55.00	501.0
55.90	2521.0
56.90	4614.0
57.90	218.0
58.80	110.0
59.90	1441.0
60.90	7187.0
61.90	7375.0
63.00	5682.0
63.90	497.0
64.80	426.0
66.90	406.0
67.90	15386.0
68.90	15097.0
69.90	1165.0
71.00	151.0
71.90	812.0
73.00	6672.0
73.90	25832.0
75.00	68512.0
75.90	6085.0
77.00	958.0
77.80	651.0
78.80	4935.0
79.80	1482.0
80.80	5140.0
81.80	1218.0
82.70	177.0
83.90	135.0
85.10	131.0
85.80	174.0
86.90	6507.0
87.90	5497.0
90.90	644.0
91.90	3763.0
92.90	5952.0
93.90	15476.0
94.90	124064.0
96.00	7942.0
96.90	309.0
102.60	151.0
103.80	639.0
104.90	254.0
105.90	795.0
106.80	158.0
108.20	106.0
110.60	154.0
111.90	238.0
112.80	189.0
114.70	178.0
115.80	499.0
116.80	1010.0
117.80	656.0
118.80	662.0
121.60	105.0
127.80	371.0
128.80	238.0
129.80	622.0
130.70	263.0
134.80	241.0
136.80	284.0
138.80	134.0
139.80	103.0
140.80	1580.0
141.60	247.0
142.90	1497.0
144.70	220.0
145.80	214.0
147.80	327.0
148.90	137.0
149.70	234.0

Instrument :
MSVOA_V
ClientSampleId :
BFB393

152.90	104.0
154.80	309.0
156.10	144.0
156.80	221.0
158.70	156.0
160.70	107.0
170.60	183.0
173.90	88272.0
174.90	7598.0
175.90	86856.0
176.90	5626.0
177.80	262.0

Instrument :
MSVOA_V
ClientSampleId :
BFB393

m/z	Abundance
35.90	1510.0
36.90	7386.0
37.90	6792.0
38.90	2670.0
39.80	1291.0
40.80	165.0
42.30	177.0
42.80	214.0
43.90	1538.0
44.90	1456.0
45.90	219.0
47.00	1874.0
47.90	1088.0
48.90	6132.0
49.90	27664.0
50.90	8612.0
51.90	386.0
52.70	122.0
53.60	114.0
54.00	124.0
54.90	405.0
55.90	2246.0
56.90	4296.0
57.90	252.0
58.70	121.0
59.90	1365.0
60.90	6628.0
61.90	6822.0
63.00	5133.0
63.90	464.0
64.90	456.0
65.90	112.0
66.90	348.0
67.90	13983.0
68.90	13690.0
69.90	1093.0
71.00	155.0
71.80	672.0
72.90	6216.0
73.90	23360.0
75.00	61912.0
75.90	5562.0
76.90	836.0
77.80	576.0
78.80	4414.0
79.80	1271.0
80.80	4655.0
81.80	1071.0
82.80	177.0
83.90	138.0
84.60	133.0
85.10	130.0
86.90	5829.0
87.90	5046.0
90.90	592.0
91.90	3561.0
93.00	5575.0
93.90	14234.0
94.90	112992.0
96.00	7386.0
96.90	307.0
100.60	125.0
102.60	132.0
103.80	611.0
104.90	218.0
105.90	773.0
106.80	147.0
108.20	129.0
110.60	182.0
112.00	239.0
112.90	171.0
114.60	186.0
115.80	439.0
116.80	904.0
117.80	530.0
118.80	591.0
121.60	106.0
123.70	114.0
127.80	370.0
128.80	234.0
129.80	533.0
130.70	270.0
134.80	198.0
136.80	247.0
138.80	134.0
139.70	116.0
140.90	1327.0
141.70	225.0
141.90	196.0
142.90	1405.0
143.80	104.0
144.70	202.0

Instrument :
MSVOA_V
ClientSampleId :
BFB393

145.80	209.0
147.80	284.0
148.90	122.0
149.70	176.0
152.90	142.0
154.80	303.0
156.00	140.0
156.80	206.0
158.80	154.0
170.60	203.0
173.90	83024.0
174.90	6818.0
175.90	79976.0
176.90	5277.0
177.80	204.0

Instrument :
MSVOA_V
ClientSampleId :
BFB393