

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102918\
 Data File : VV008461.D
 Acq On : 29 Oct 2018 18:11
 Operator : SY/MD
 Sample : J5716-10
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBX7

Quant Time: Oct 30 08:55:11 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 30 07:40:49 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	180244	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	163931	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	66834	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	43880	43.97	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	87.94%
7) Chloroethane-d5	1.56	69	35071	48.67	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	97.34%
11) 1,1-Dichloroethene-d2	2.13	63	62438	34.64	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.28%
21) 2-Butanone-d5	3.94	46	106394	98.10	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	98.10%
24) Chloroform-d	4.41	84	115564	46.95	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.90%
26) 1,2-Dichloroethane-d4	5.09	65	81716	49.66	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.32%
32) Benzene-d6	5.10	84	236393	50.60	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.20%
36) 1,2-Dichloropropane-d6	6.12	67	81697	50.38	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.76%
41) Toluene-d8	7.36	98	210867	49.71	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.42%
43) trans-1,3-Dichloropropene-	7.67	79	38495	48.86	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	97.72%
47) 2-Hexanone-d5	8.14	63	81034	95.71	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	95.71%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	111199	50.63	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	101.26%
64) 1,2-Dichlorobenzene-d4	11.68	152	70738	51.74	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.48%


Target Compounds					Qvalue
13) Acetone	2.19	43	4006	4.76 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102918\
Data File : VV008461.D
Acq On : 29 Oct 2018 18:11
Operator : SY/MD
Sample : J5716-10
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETBX7

Quant Time: Oct 30 08:55:11 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 30 07:40:49 2018
Response via : Initial Calibration

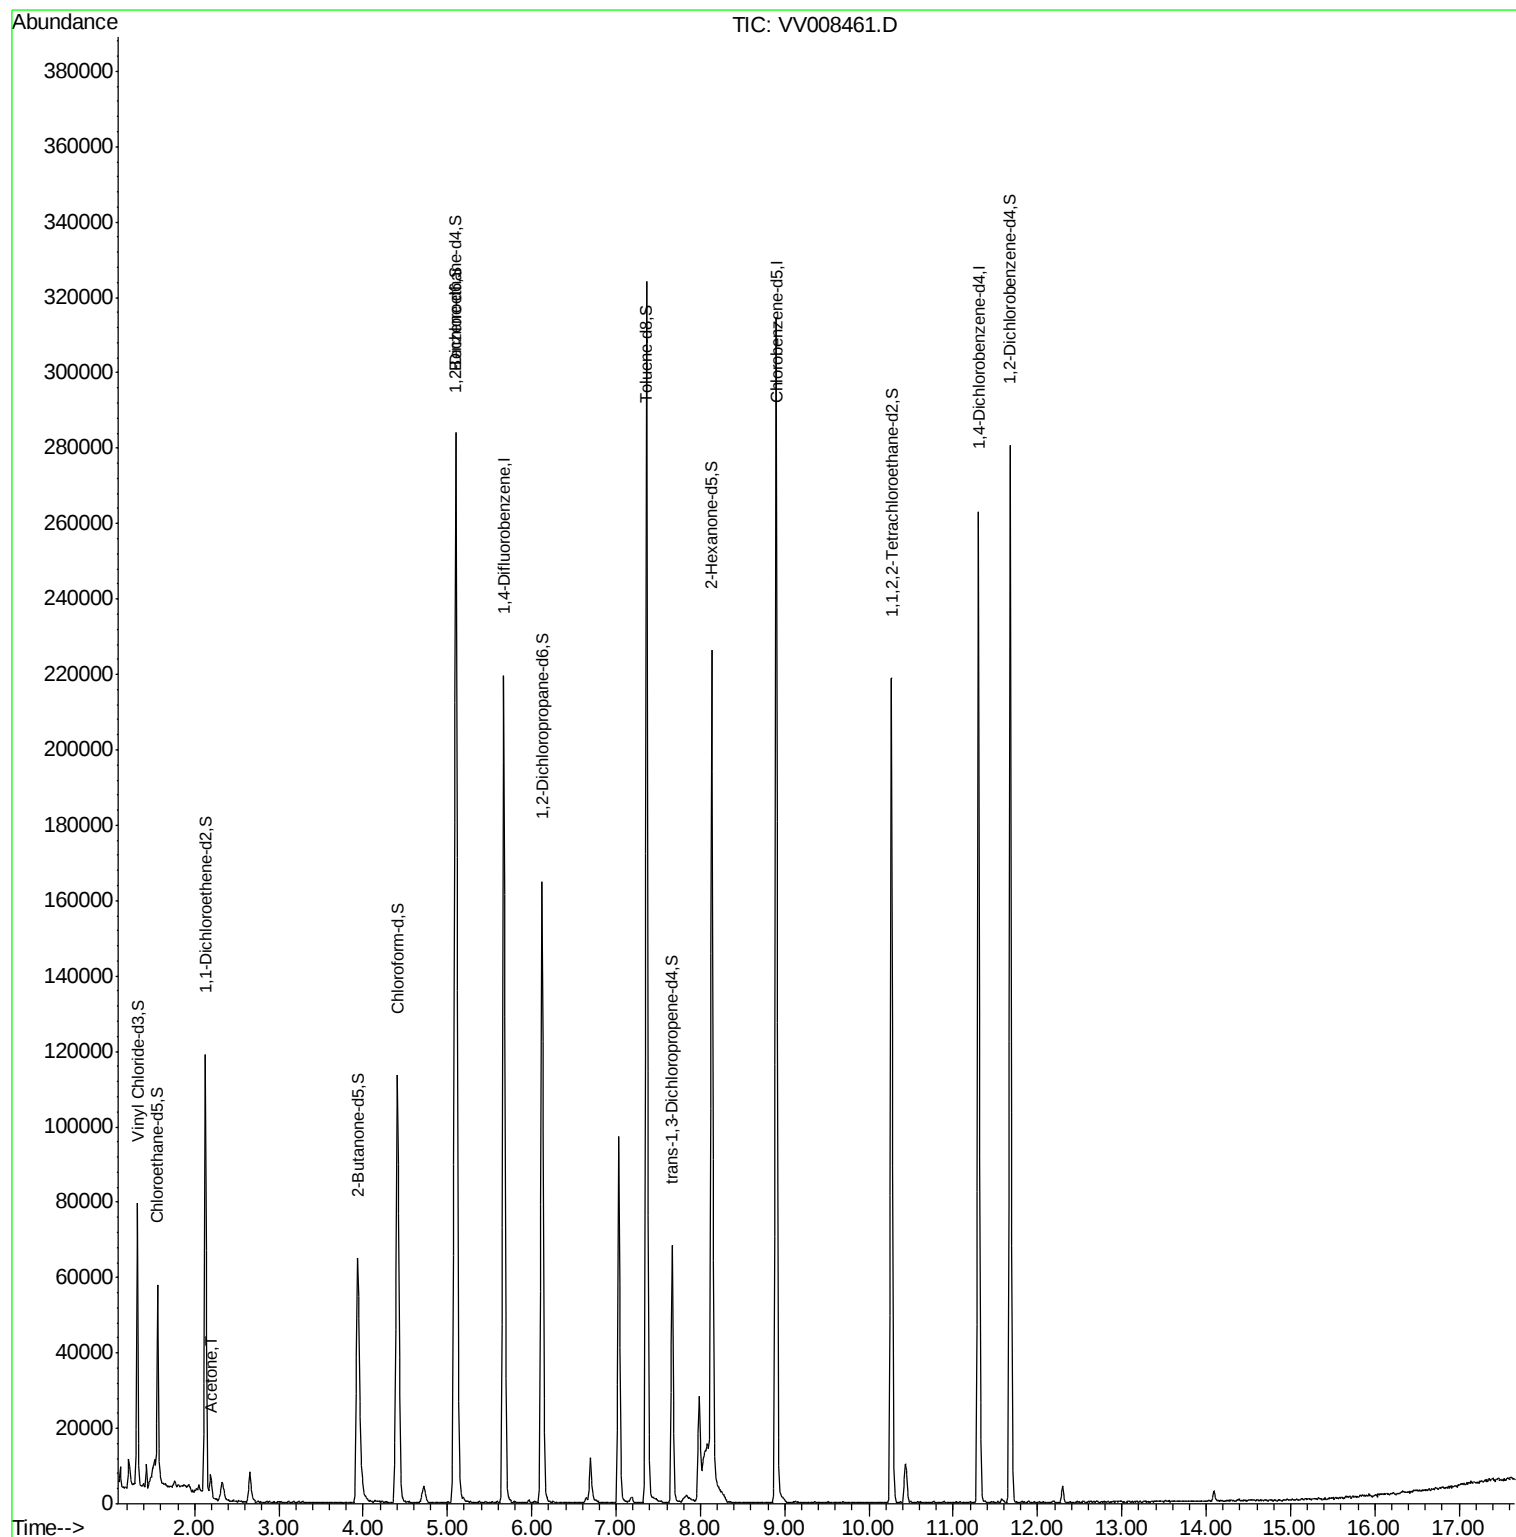

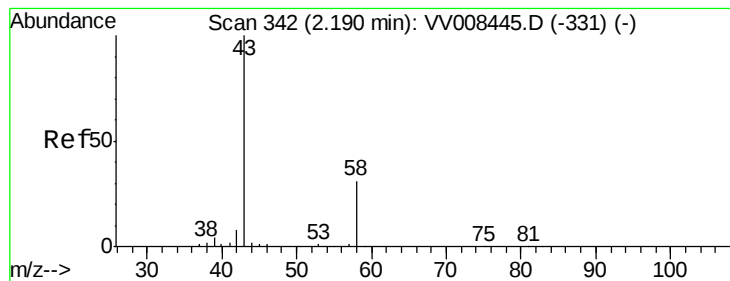

#13
 Acetone
 Concen: 4.76 ug/L
 RT: 2.19 min Scan# 343
 Delta R.T. 0.00 min
 Lab File: VV008461.D
 Acq: 29 Oct 2018 18:11

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBX7

Tgt Ion: 43 Resp: 4006
 Ion Ratio Lower Upper
 43 100
 58 30.0 0.0 61.4

