

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102918\
 Data File : VV008462.D
 Acq On : 29 Oct 2018 18:35
 Operator : SY/MD
 Sample : J5716-11
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBY0

Quant Time: Oct 30 08:57:26 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 30 07:40:49 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	176379	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	158447	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	64971	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	42987	44.02	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	88.04%
7) Chloroethane-d5	1.56	69	34600	49.07	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	98.14%
11) 1,1-Dichloroethene-d2	2.13	63	59890	33.95	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.90%
21) 2-Butanone-d5	3.94	46	105591	99.49	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.49%
24) Chloroform-d	4.41	84	114966	47.73	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.46%
26) 1,2-Dichloroethane-d4	5.09	65	79317	49.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.50%
32) Benzene-d6	5.10	84	231062	51.17	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.34%
36) 1,2-Dichloropropane-d6	6.12	67	79409	50.67	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.34%
41) Toluene-d8	7.36	98	205301	50.08	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.16%
43) trans-1,3-Dichloropropene-	7.67	79	38044	49.96	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	99.92%
47) 2-Hexanone-d5	8.14	63	79575	97.23	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	97.23%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	109542	51.61	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	103.22%
64) 1,2-Dichlorobenzene-d4	11.68	152	70868	53.32	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.64%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	2.19	43	6296	7.64	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102918\
 Data File : VV008462.D
 Acq On : 29 Oct 2018 18:35
 Operator : SY/MD
 Sample : J5716-11
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 ETBY0

Quant Time: Oct 30 08:57:26 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 30 07:40:49 2018
 Response via : Initial Calibration

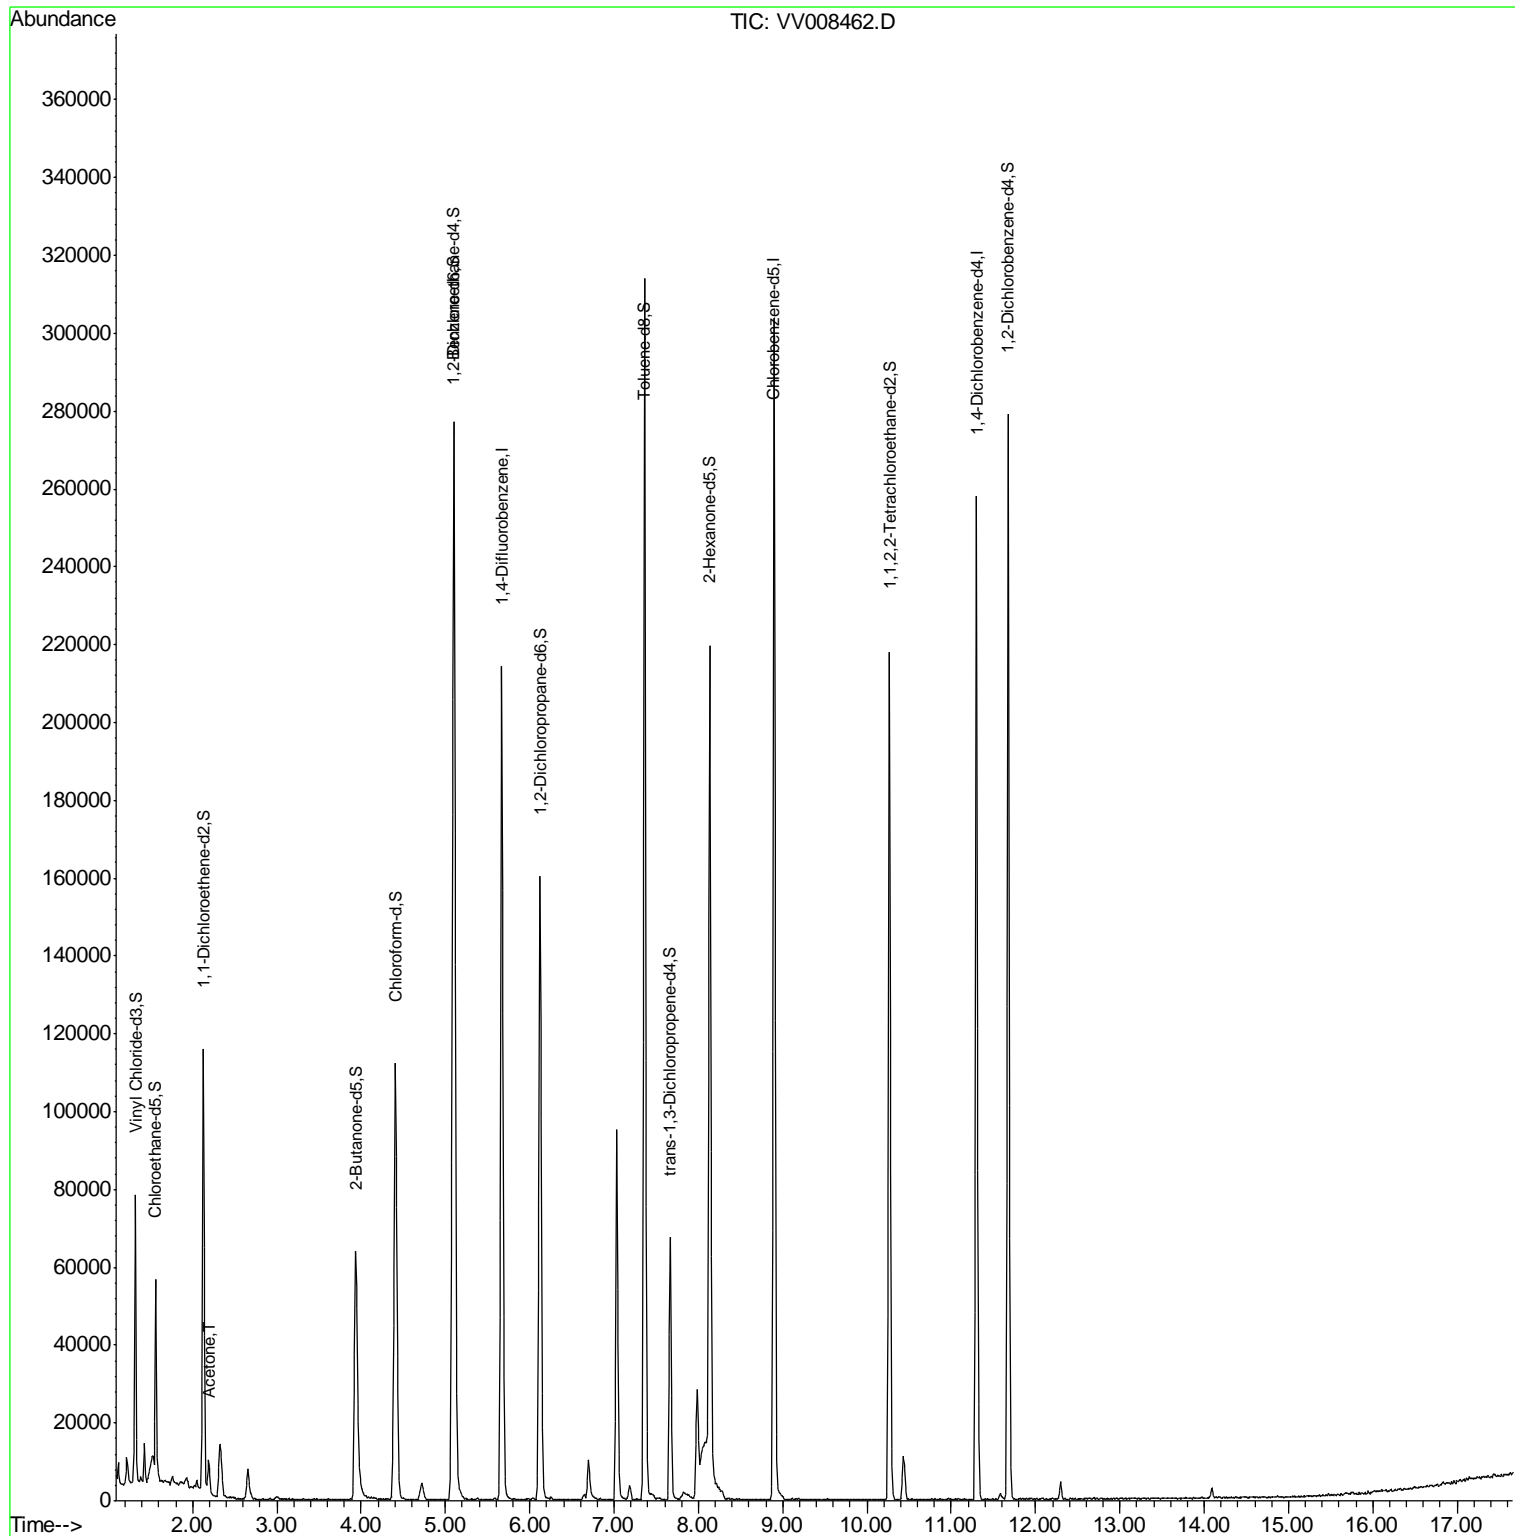

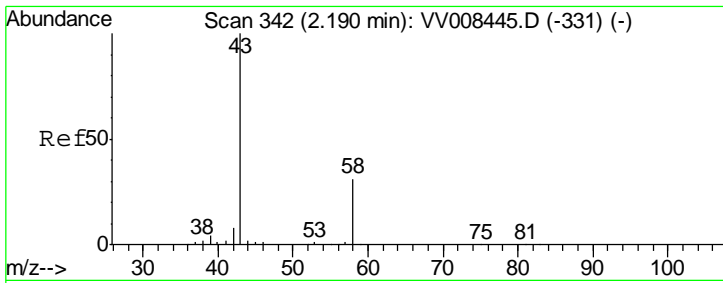

#13
 Acetone
 Concen: 7.64 ug/L
 RT: 2.19 min Scan# 343
 Delta R.T. 0.00 min
 Lab File: VV008462.D
 Acq: 29 Oct 2018 18:35

Instrument :
 MSVOA_V
ClientSampled :
 ETBY0

Tgt Ion: 43 Resp: 6296

Ion	Ratio	Lower	Upper
43	100		
58	32.5	0.0	61.4

