

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102918\
 Data File : VV008464.D
 Acq On : 29 Oct 2018 19:21
 Operator : SY/MD
 Sample : J5716-09
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBX6

Quant Time: Oct 30 09:04:11 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 30 07:40:49 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	184284	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	166637	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	68784	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	44293	43.41	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.82%
7) Chloroethane-d5	1.56	69	35727	48.50	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	97.00%
11) 1,1-Dichloroethene-d2	2.13	63	61833	33.55	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.10%
21) 2-Butanone-d5	3.93	46	108626	97.96	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.96%
24) Chloroform-d	4.41	84	119329	47.42	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.84%
26) 1,2-Dichloroethane-d4	5.09	65	84083	49.97	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.94%
32) Benzene-d6	5.10	84	238218	50.17	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.34%
36) 1,2-Dichloropropane-d6	6.12	67	82710	50.18	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.36%
41) Toluene-d8	7.36	98	213216	49.45	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.90%
43) trans-1,3-Dichloropropene-	7.67	79	39520	49.35	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	98.70%
47) 2-Hexanone-d5	8.14	63	80466	93.49	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.49%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	110874	49.67	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	99.34%
64) 1,2-Dichlorobenzene-d4	11.68	152	71597	50.89	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.78%


Target Compounds					Qvalue
13) Acetone	2.19	43	5234	6.08 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102918\
Data File : VV008464.D
Acq On : 29 Oct 2018 19:21
Operator : SY/MD
Sample : J5716-09
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETBX6

Quant Time: Oct 30 09:04:11 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 30 07:40:49 2018
Response via : Initial Calibration

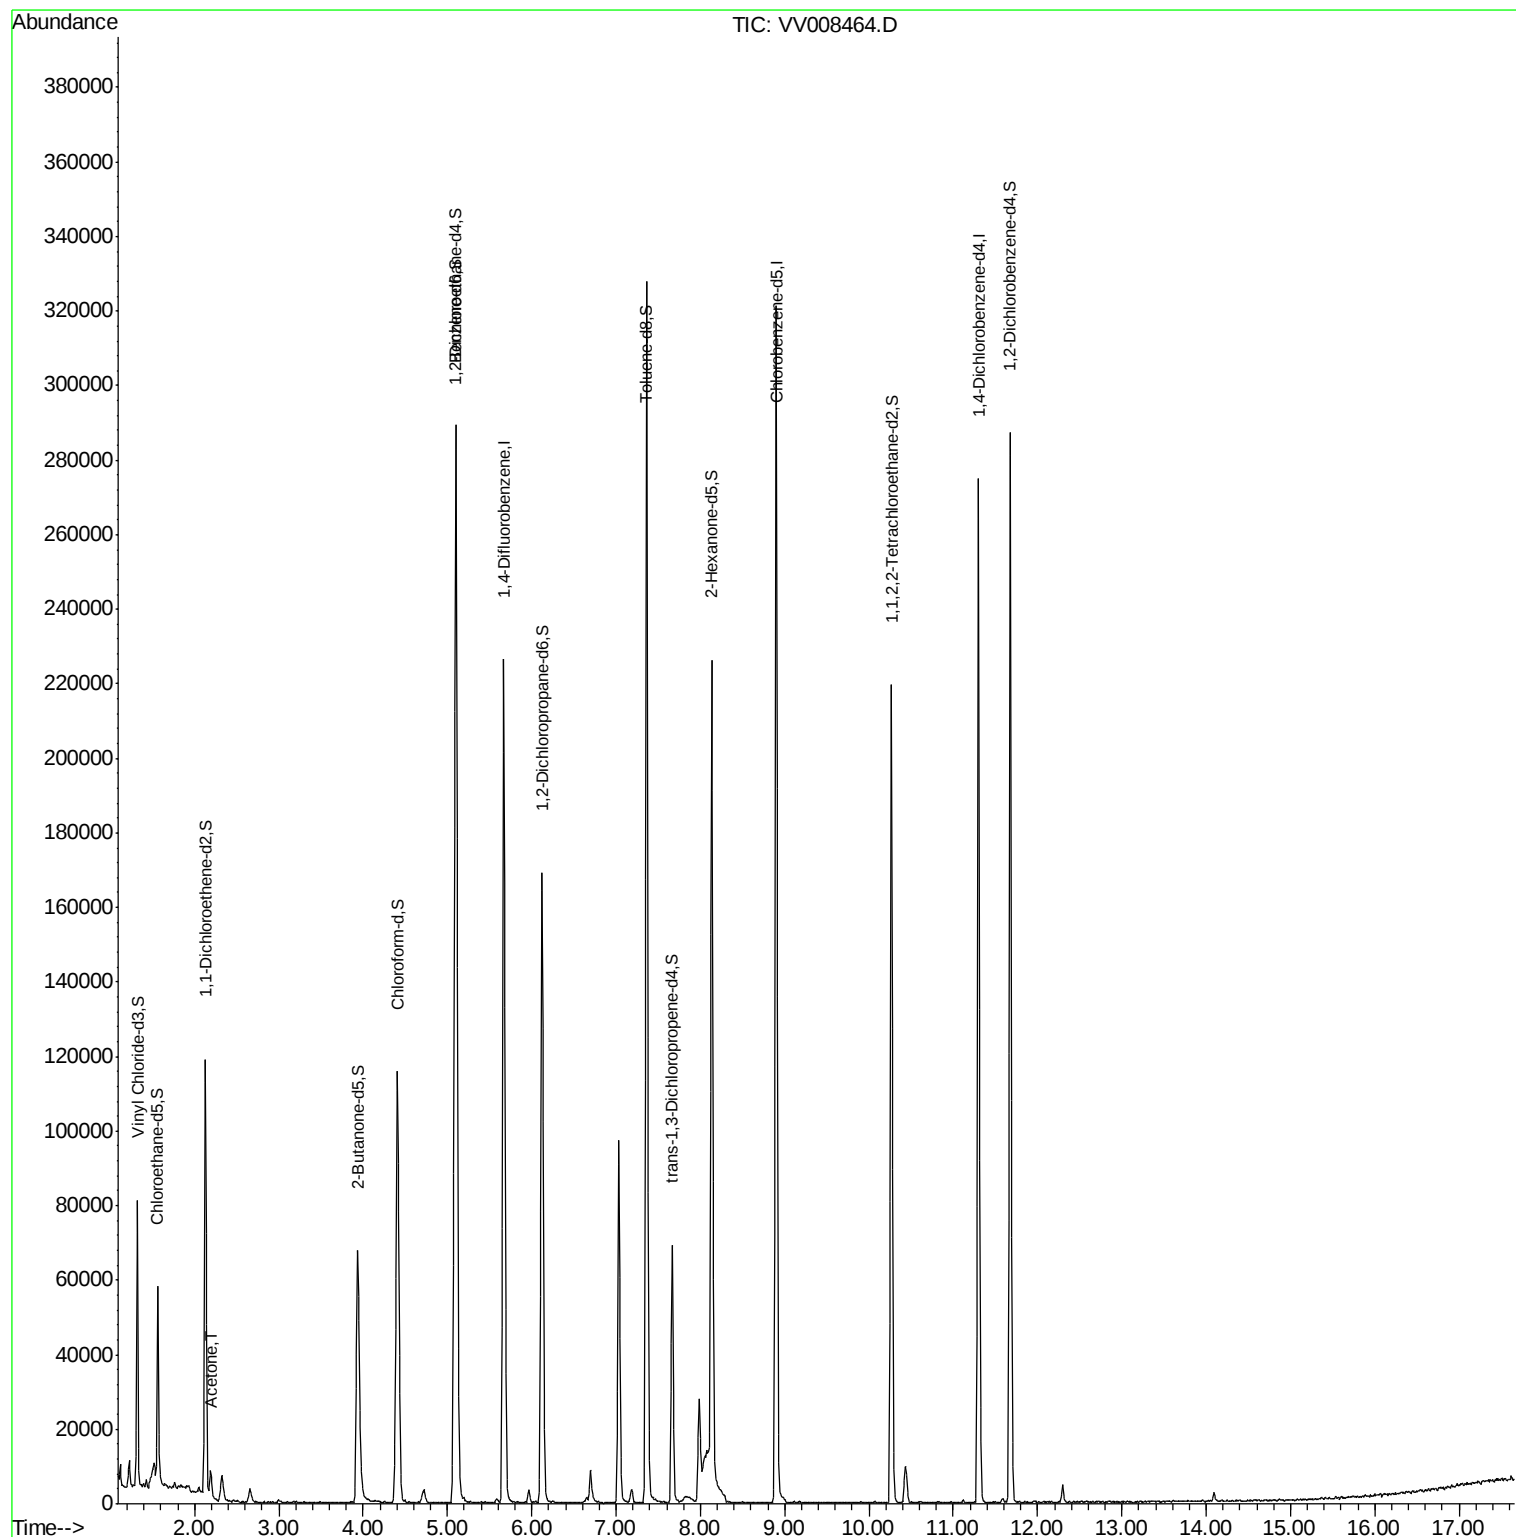

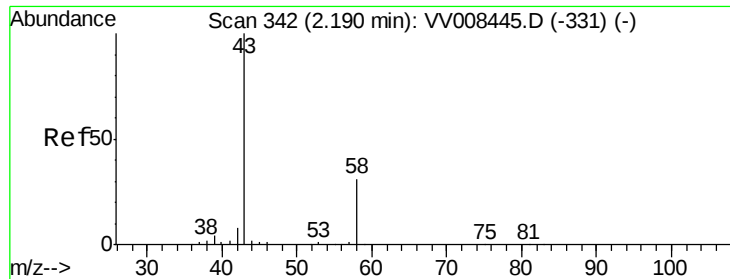

#13

Acetone

Concen: 6.08 ug/L

RT: 2.19 min Scan# 343

Delta R.T. 0.00 min

Lab File: VV008464.D

Acq: 29 Oct 2018 19:21

Instrument :
MSVOA_V
ClientSampleId :
ETBX6

Tgt Ion: 43 Resp: 5234

Ion Ratio Lower Upper

43 100

58 31.8 0.0 61.4

