


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102918\
 Data File : VV008444.D
 Acq On : 29 Oct 2018 10:43
 Operator : SY/MD
 Sample : BFB52
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB52

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
 Title : VOC Analysis
 Last Update : Tue Oct 30 07:40:49 2018

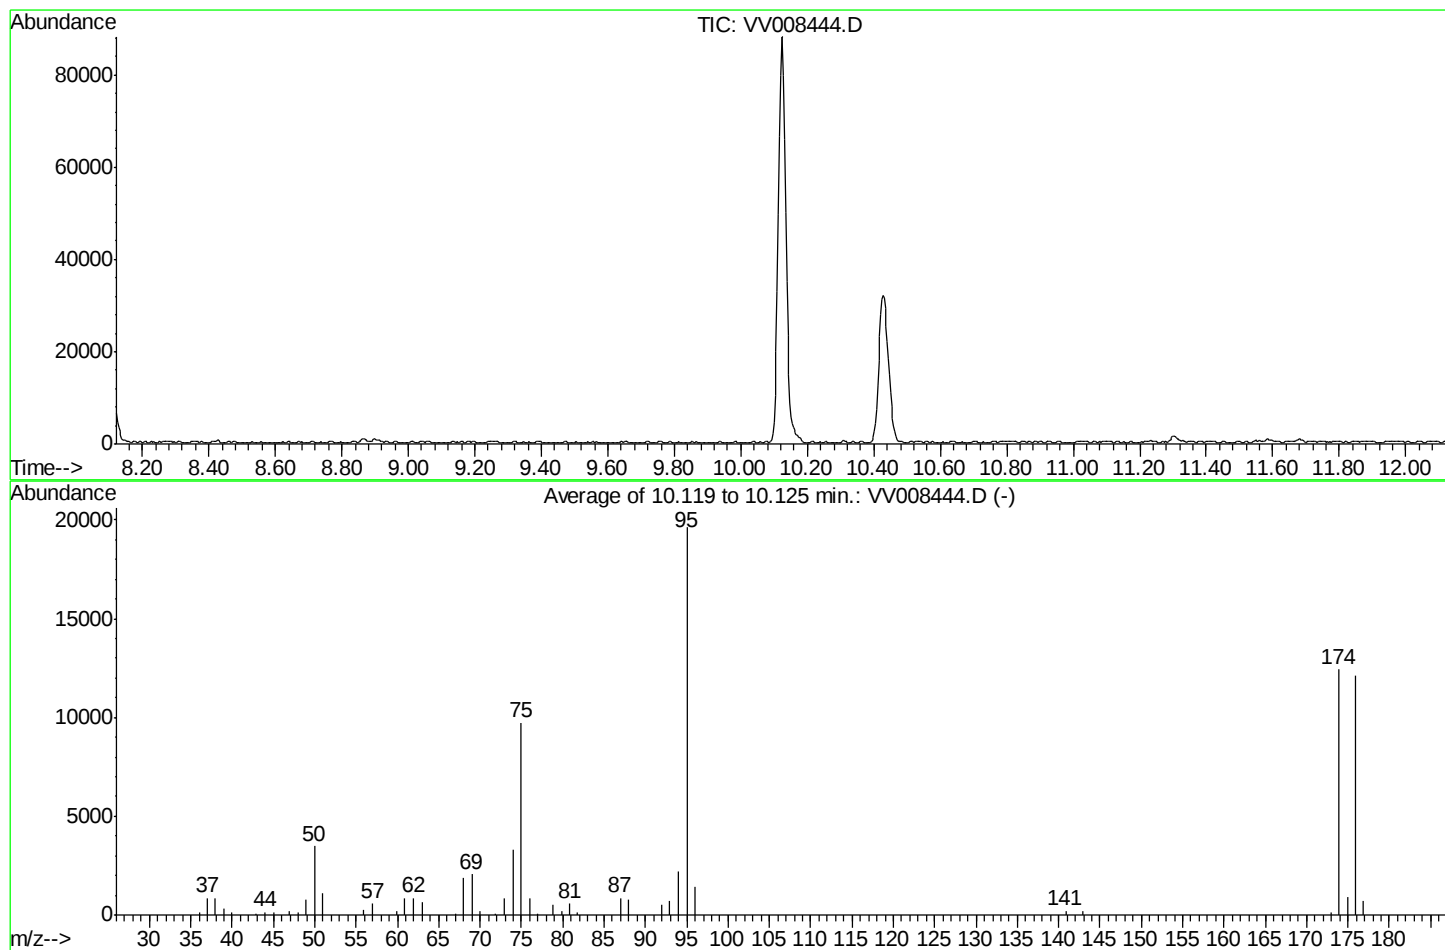

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	3495	PASS
75	95	30	80	49.6	9728	PASS
95	95	100	100	100.0	19626	PASS
96	95	5	9	7.3	1435	PASS
173	174	0.00	2	1.1	131	PASS
174	95	50	120	63.4	12438	PASS
175	174	5	9	7.2	901	PASS
176	174	95	101	97.7	12151	PASS
177	176	5	9	6.1	740	PASS

m/z	Abundance
36.00	151.0
37.00	883.0
37.90	856.0
39.00	357.0
39.90	133.0
43.00	101.0
44.00	438.0
45.00	150.0
46.90	205.0
47.90	131.0
49.00	786.0
50.00	3602.0
51.00	1190.0
55.90	233.0
57.00	572.0
59.90	221.0
60.90	855.0
62.00	858.0
63.00	664.0
68.00	1954.0
69.00	2114.0
69.90	191.0
71.90	127.0
73.00	886.0
74.00	3458.0
75.00	10011.0
76.00	851.0
76.90	108.0
78.80	536.0
79.90	189.0
80.90	599.0
81.80	132.0
86.90	857.0
87.90	830.0
91.90	563.0
92.90	753.0
94.00	2314.0
95.00	20272.0
96.00	1466.0
140.90	216.0
142.80	199.0
172.90	131.0
173.90	12766.0
174.90	917.0
175.90	12558.0
176.90	757.0

Instrument :
MSVOA_V
ClientSampleId :
BFB52

m/z	Abundance
36.00	147.0
37.00	821.0
37.90	875.0
39.00	366.0
39.90	122.0
42.90	102.0
44.00	500.0
45.00	159.0
46.90	239.0
47.90	125.0
48.90	795.0
50.00	3455.0
51.00	1097.0
55.90	225.0
57.00	491.0
59.90	205.0
60.90	907.0
62.00	883.0
63.00	698.0
68.00	1937.0
69.00	2178.0
70.00	192.0
71.90	125.0
73.00	922.0
74.00	3437.0
75.00	10043.0
76.00	768.0
76.90	120.0
78.80	526.0
79.90	198.0
80.90	551.0
81.80	119.0
86.90	895.0
87.90	786.0
91.90	545.0
93.00	732.0
94.00	2276.0
95.00	20208.0
96.00	1421.0
140.90	231.0
142.80	178.0
172.90	118.0
173.90	12966.0
174.90	931.0
175.90	12822.0
176.90	796.0

Instrument :
MSVOA_V
ClientSampleId :
BFB52

m/z	Abundance
36.00	151.0
37.00	849.0
37.90	749.0
39.00	332.0
39.90	133.0
44.00	361.0
45.00	139.0
46.90	190.0
48.00	130.0
49.00	734.0
50.00	3430.0
51.00	1120.0
55.90	237.0
57.00	630.0
59.90	204.0
60.90	759.0
61.90	824.0
63.00	608.0
67.10	116.0
68.00	1766.0
69.00	1847.0
69.90	189.0
72.90	782.0
74.00	3072.0
75.00	9130.0
76.00	831.0
78.80	504.0
80.00	151.0
80.80	521.0
81.80	143.0
87.00	777.0
87.90	786.0
92.00	509.0
93.00	716.0
94.00	2120.0
95.00	18400.0
96.00	1419.0
140.90	165.0
142.90	180.0
172.90	144.0
174.00	11582.0
175.00	855.0
175.90	11073.0
176.90	669.0

Instrument :
MSVOA_V
ClientSampleId :
BFB52

m/z	Abundance
44.00	271.0

Instrument :
MSVOA_V
ClientSampleId :
BFB52