


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV102919\
 Data File : VV013389.D
 Acq On : 29 Oct 2019 10:03
 Operator : SY/MD
 Sample : BFB51
 Misc : 25.0ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB51

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102919WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Nov 04 07:24:15 2019

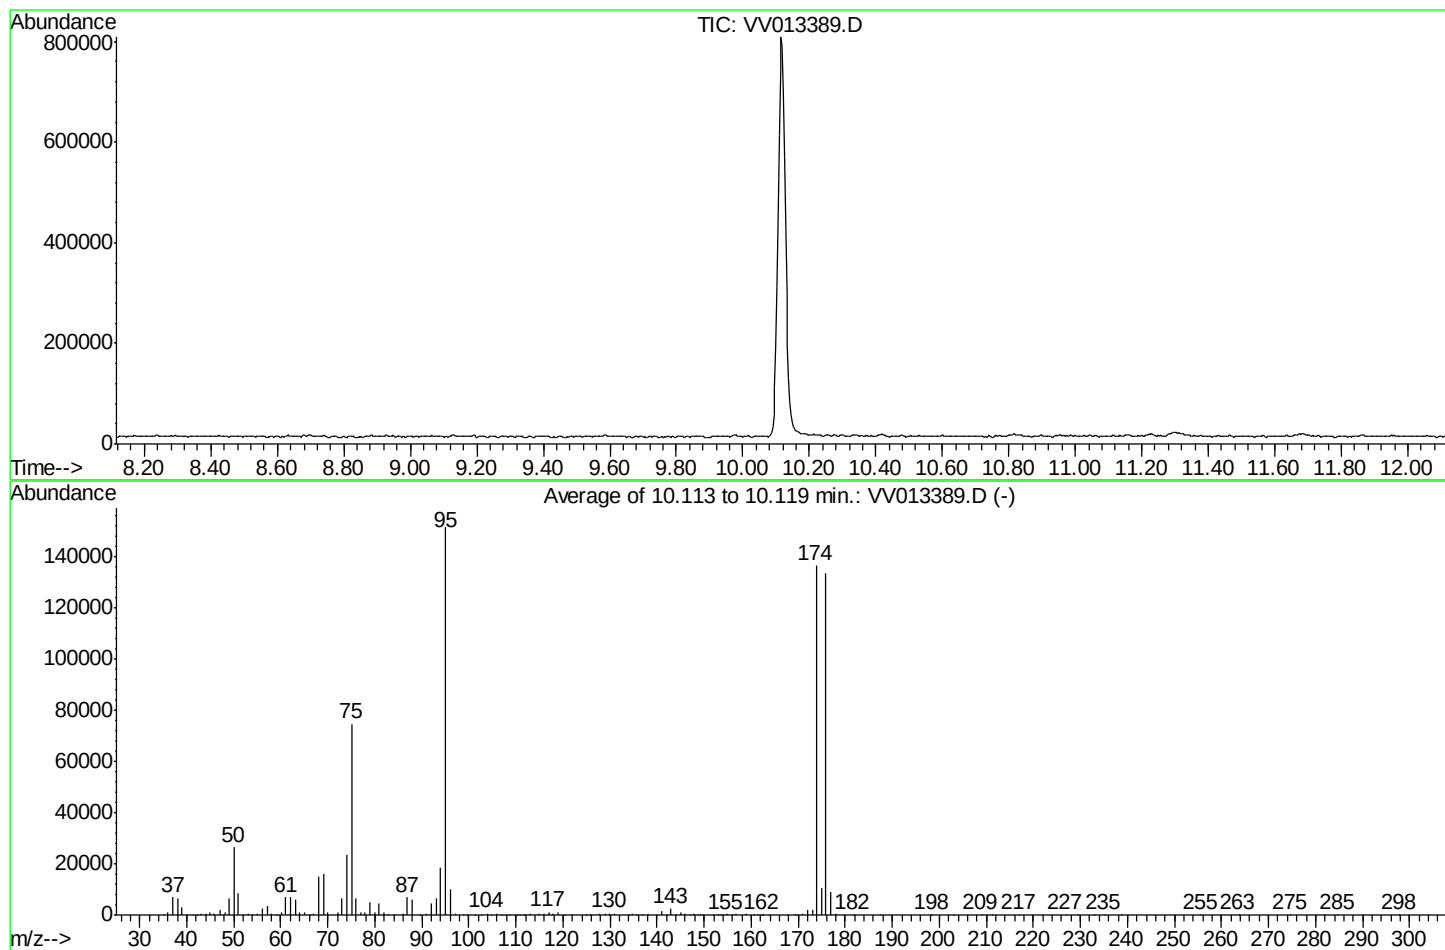

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	26422	PASS
75	95	30	80	49.3	74621	PASS
95	95	100	100	100.0	151466	PASS
96	95	5	9	6.8	10253	PASS
173	174	0.00	2	1.6	2136	PASS
174	95	50	120	90.1	136501	PASS
175	174	5	9	7.8	10586	PASS
176	174	95	101	97.9	133690	PASS
177	176	5	9	6.7	8972	PASS

m/z	Abundance
35.10	211.0
36.00	1392.0
37.10	6557.0
38.00	6300.0
39.00	3282.0
40.00	1540.0
40.80	279.0
41.30	240.0
41.90	199.0
43.00	298.0
44.10	2003.0
45.00	1301.0
46.00	427.0
47.00	1846.0
48.20	961.0
49.00	6566.0
50.00	25344.0
51.10	8522.0
52.00	365.0
53.00	367.0
53.90	211.0
55.00	487.0
56.00	2431.0
57.10	3259.0
58.30	211.0
59.10	133.0
60.00	1193.0
61.00	7048.0
62.00	6860.0
63.10	5971.0
64.00	1326.0
65.10	1276.0
65.90	236.0
67.00	505.0
68.00	14752.0
69.00	15298.0
70.00	1141.0
72.00	1035.0
73.10	6038.0
74.00	22784.0
75.00	71560.0
76.00	6175.0
77.10	942.0
77.80	942.0
78.90	4575.0
79.90	1087.0
80.90	4400.0
82.00	947.0
82.80	199.0
84.20	178.0
85.90	533.0
86.90	6558.0
87.90	5908.0
90.90	726.0
92.00	4374.0
93.00	6314.0
94.00	17736.0
95.00	145152.0
96.00	10016.0
97.20	336.0
98.80	121.0
101.10	122.0
102.70	262.0
103.90	650.0
104.80	316.0
105.90	478.0
107.10	189.0
108.70	182.0
109.80	123.0
110.20	139.0
110.70	199.0
111.90	194.0
112.90	323.0
114.80	332.0
116.00	578.0
116.90	1120.0
117.80	600.0
119.00	1096.0
120.40	167.0
121.80	160.0
124.90	117.0
125.60	146.0
126.00	150.0
127.70	533.0
129.00	284.0
129.90	588.0
130.90	293.0
133.80	107.0
134.80	344.0
136.90	314.0
139.90	250.0
140.90	1191.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51

142.00	328.0
142.90	2002.0
145.10	980.0
145.90	374.0
147.10	113.0
147.70	451.0
148.70	145.0
149.20	116.0
149.80	112.0
151.90	187.0
152.90	243.0
153.40	111.0
154.00	242.0
154.90	520.0
155.90	120.0
156.80	388.0
158.80	272.0
161.20	182.0
162.10	102.0
163.90	100.0
169.20	104.0
170.90	454.0
172.10	1995.0
173.00	2010.0
173.90	127328.0
175.00	10035.0
175.90	124592.0
177.00	8152.0
177.90	258.0
187.50	111.0
198.50	116.0
203.10	110.0
208.90	139.0
217.00	108.0
233.00	118.0
235.00	111.0
255.60	152.0
263.60	131.0
281.90	117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51

m/z	Abundance
35.10	262.0
35.90	1402.0
37.10	7077.0
38.00	6828.0
39.00	3304.0
40.00	1604.0
41.30	210.0
41.90	188.0
42.20	170.0
43.00	308.0
44.00	1702.0
45.00	1319.0
45.80	445.0
47.00	2024.0
48.10	977.0
49.00	6692.0
50.00	27352.0
51.10	8959.0
52.00	423.0
53.10	431.0
54.00	191.0
55.10	503.0
56.00	2328.0
57.00	3543.0
58.10	258.0
60.00	1315.0
61.00	7134.0
62.00	7387.0
63.10	6470.0
64.00	1359.0
65.10	1308.0
66.10	280.0
67.00	622.0
68.00	15581.0
69.00	16752.0
70.00	1249.0
70.80	162.0
72.00	921.0
73.00	6784.0
74.00	24744.0
75.00	77448.0
76.00	6729.0
77.10	1091.0
77.80	979.0
78.90	5112.0
79.90	1179.0
80.90	4738.0
81.90	923.0
82.80	198.0
84.20	182.0
86.00	521.0
86.90	7042.0
87.90	6265.0
90.90	715.0
92.00	4740.0
93.00	6774.0
94.00	19512.0
95.00	157248.0
96.00	10602.0
97.10	352.0
98.70	105.0
101.10	130.0
102.70	237.0
103.90	609.0
104.80	250.0
105.90	502.0
107.10	154.0
107.80	125.0
108.70	203.0
109.70	132.0
110.20	167.0
110.80	218.0
111.80	173.0
112.90	319.0
114.80	297.0
116.00	618.0
116.90	1203.0
117.90	646.0
119.00	1117.0
120.40	108.0
125.60	108.0
126.00	163.0
127.70	636.0
128.90	342.0
129.90	702.0
130.90	297.0
134.80	275.0
135.60	168.0
136.80	244.0
138.00	111.0
139.90	213.0
140.90	1310.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51

141.90	302.0
143.00	2513.0
144.00	202.0
145.00	1228.0
146.00	364.0
147.00	162.0
147.70	482.0
149.20	156.0
152.90	257.0
153.40	122.0
154.00	182.0
154.80	510.0
156.80	473.0
158.90	360.0
160.70	159.0
161.30	160.0
162.40	121.0
167.80	101.0
169.10	109.0
169.90	107.0
171.00	577.0
172.00	2151.0
173.00	2208.0
173.90	141504.0
175.00	10823.0
175.90	138496.0
177.00	9391.0
177.90	292.0
181.70	108.0
207.10	105.0
208.90	136.0
226.90	103.0
235.00	102.0
238.60	103.0
255.50	173.0
263.60	104.0
284.80	111.0
297.80	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51

m/z	Abundance
35.00	278.0
35.90	1307.0
37.10	7080.0
38.00	6775.0
39.00	3053.0
40.00	1581.0
41.20	146.0
42.20	214.0
43.00	251.0
44.00	1585.0
45.00	1291.0
45.80	416.0
47.00	2168.0
48.10	1036.0
49.00	6092.0
50.00	27088.0
51.00	8543.0
52.00	428.0
53.10	415.0
53.80	195.0
55.10	479.0
56.00	2121.0
57.00	3496.0
58.00	371.0
60.10	1282.0
61.00	6699.0
62.00	6912.0
63.00	6276.0
63.90	1201.0
65.00	1438.0
66.10	312.0
67.00	653.0
68.00	14733.0
69.00	16001.0
70.10	1304.0
70.80	177.0
72.00	860.0
73.00	6531.0
74.00	23960.0
75.00	74856.0
76.00	6413.0
77.10	1162.0
77.80	889.0
78.90	5052.0
79.90	1216.0
80.90	4606.0
81.90	844.0
82.90	161.0
84.30	157.0
86.00	496.0
87.00	6844.0
88.00	6220.0
89.50	154.0
90.20	122.0
90.80	710.0
92.00	4541.0
93.00	6750.0
94.00	18680.0
95.00	152000.0
96.00	10141.0
97.10	400.0
99.50	126.0
101.20	134.0
102.70	191.0
103.90	526.0
104.90	238.0
105.90	542.0
107.10	132.0
107.90	192.0
108.70	145.0
109.70	148.0
110.30	163.0
110.80	215.0
111.60	178.0
112.80	279.0
114.90	244.0
116.00	570.0
117.00	1125.0
117.90	626.0
119.00	914.0
126.10	187.0
127.70	636.0
128.90	351.0
129.90	710.0
130.90	285.0
134.80	257.0
135.60	187.0
136.70	218.0
140.90	1371.0
141.90	226.0
143.00	2753.0
144.00	248.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51

145.00	1243.0
146.00	315.0
147.00	192.0
147.80	414.0
149.20	158.0
152.90	234.0
153.50	104.0
153.90	106.0
154.80	454.0
156.90	428.0
158.90	386.0
160.70	159.0
161.30	135.0
162.30	124.0
167.70	148.0
169.10	120.0
169.90	163.0
171.00	561.0
171.90	1988.0
173.00	2191.0
173.90	140672.0
175.00	10900.0
175.90	137984.0
177.00	9375.0
178.00	322.0
181.70	104.0
198.10	101.0
207.10	224.0
211.20	118.0
229.30	105.0
255.50	112.0
274.70	135.0
284.70	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51

m/z	Abundance
35.30	256.0
36.00	407.0
37.40	190.0
38.70	161.0
40.00	1479.0
40.70	119.0
41.80	151.0
42.70	170.0
44.00	1404.0
45.00	195.0
45.80	140.0
46.10	140.0
47.20	154.0
47.60	171.0
47.80	176.0
49.20	163.0
50.00	172.0
50.90	196.0
51.60	117.0
52.20	186.0
53.60	119.0
54.80	143.0
55.70	224.0
56.30	173.0
57.60	157.0
59.70	158.0
62.00	109.0
62.30	119.0
63.30	126.0
64.00	167.0
65.10	184.0
65.20	183.0
65.90	161.0
66.90	118.0
69.60	102.0
70.80	221.0
71.60	231.0
72.10	130.0
73.90	164.0
77.20	128.0
80.90	112.0
81.80	119.0
82.80	150.0
84.10	120.0
87.70	101.0
88.50	106.0
89.90	103.0
90.30	117.0
97.70	132.0
100.90	179.0
102.00	108.0
105.90	147.0
107.00	149.0
109.10	180.0
113.60	109.0
119.90	109.0
121.00	111.0
122.70	110.0
127.40	112.0
129.30	107.0
130.50	129.0
132.00	105.0
132.60	151.0
142.10	116.0
144.90	103.0
146.90	126.0
150.70	119.0
155.20	104.0
166.00	124.0
166.40	108.0
170.80	149.0
171.40	113.0
179.70	138.0
184.60	109.0
207.00	134.0
208.00	117.0
220.70	128.0
227.40	102.0
228.00	157.0
229.90	123.0
245.20	120.0
261.20	130.0
261.90	178.0
267.60	124.0
268.80	108.0
279.50	117.0
288.80	117.0
294.00	147.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51