

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102920\
 Data File : VV019169.D
 Acq On : 30 Oct 2020 01:09
 Operator : SY/MD
 Sample : L4502-19ME 40X
 Misc : 6.01g/5.0ml/100uL/5.0ml/MSVOA-V/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG442ME

Quant Time: Oct 30 06:19:42 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 30 05:31:22 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	225385	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	218572	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	105570	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	80182	44.77	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	89.54%
7) Chloroethane-d5	1.58	69	65366	46.98	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	93.96%
11) 1,1-Dichloroethene-d2	2.12	63	117180	34.39	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.78%
21) 2-Butanone-d5	3.91	46	112028	102.12	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	102.12%
24) Chloroform-d	4.38	84	162640	48.81	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.62%
26) 1,2-Dichloroethane-d4	5.06	65	118516	51.05	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.10%
32) Benzene-d6	5.07	84	303434	48.94	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.88%
36) 1,2-Dichloropropane-d6	6.09	67	92684	50.13	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.26%
41) Toluene-d8	7.34	98	272177	45.70	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.40%
43) trans-1,3-Dichloropropene-	7.64	79	50502	47.21	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.42%
47) 2-Hexanone-d5	8.11	63	81110	101.31	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	101.31%
57) 1,1,2,2-Tetrachloroethane-	10.23	84	123077	49.38	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.76%
64) 1,2-Dichlorobenzene-d4	11.65	152	115308	51.99	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.98%


Target Compounds					Ovalue
46) Tetrachloroethene	8.00	164	30637	20.782 ug/L	98




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102920\
Data File : VV019169.D
Acq On : 30 Oct 2020 01:09
Operator : SY/MD
Sample : L4502-19ME 40X
Misc : 6.01g/5.0ml/100uL/5.0ml/MSVOA-V/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG442ME

Quant Time: Oct 30 06:19:42 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 30 05:31:22 2020
Response via : Initial Calibration

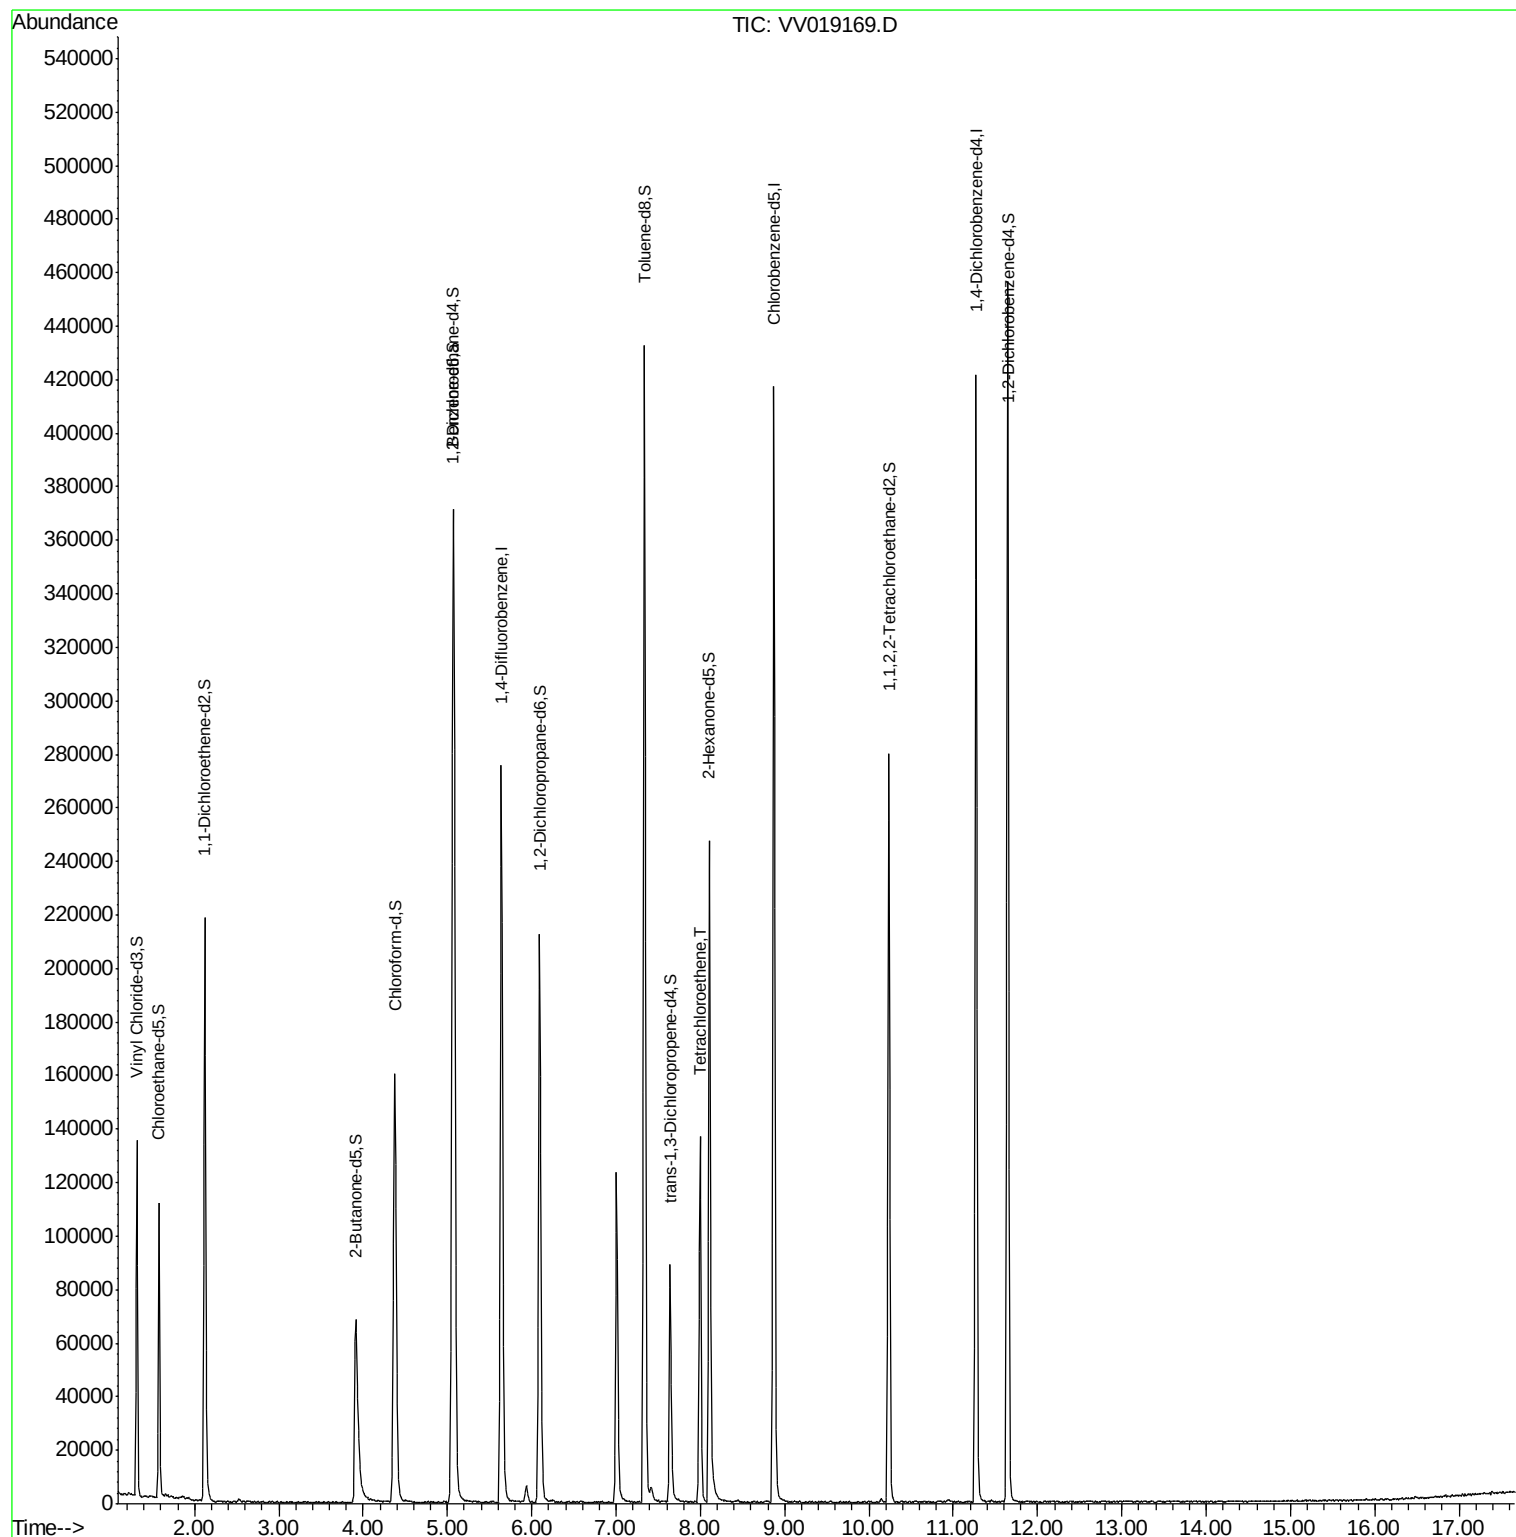

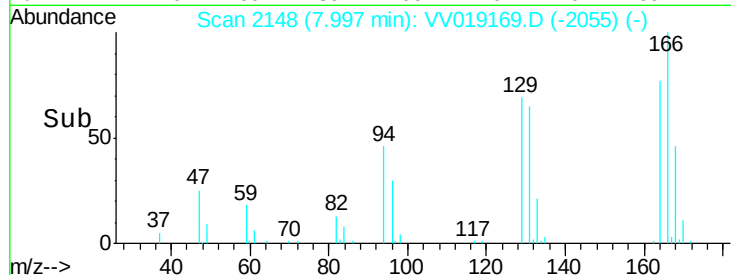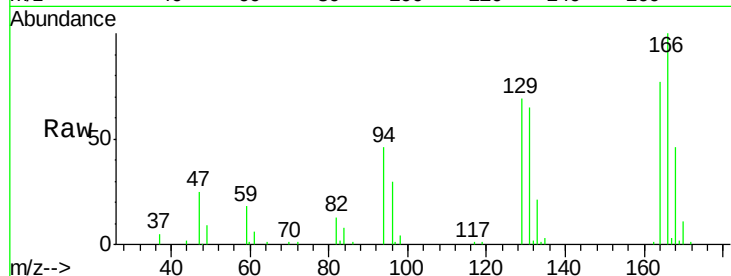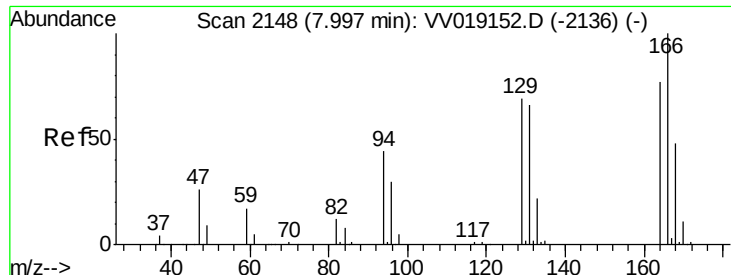

#46

Tetrachloroethene

Concen: 20.782 ug/L

RT: 8.00 min Scan# 2148

Delta R.T. -0.00 min

Lab File: VV019169.D

Acq: 30 Oct 2020 01:09

Instrument :

MSVOA_V

ClientSampleId :

BG442ME

Tot Ion:164 Resp: 30637

Ion Ratio Lower Upper

164 100

129 89.2 63.2 117.4

131 85.1 60.3 112.1

166 130.0 88.3 163.9

Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

