

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102920\
 Data File : VV019168.D
 Acq On : 30 Oct 2020 00:45
 Operator : SY/MD
 Sample : L4502-18ME 40X
 Misc : 6.04g/5.0ml/100uL/5.0ml/MSVOA-V/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG441ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	85	rVB	130813	130381	14.08%	1.764%
2	1.579	145	152	164	rVB	110832	121553	13.13%	1.644%
3	2.123	310	321	341	rBV	217049	321764	34.75%	4.352%
4	2.293	372	374	375	rBV	319	120	0.01%	0.002%
5	2.460	421	426	431	rBV2	453	553	0.06%	0.007%
6	2.640	475	482	484	rBV3	518	524	0.06%	0.007%
7	2.676	490	493	497	rBV2	301	294	0.03%	0.004%
8	2.766	518	521	524	rBV	382	275	0.03%	0.004%
9	2.785	525	527	529	rVB	167	71	0.01%	0.001%
10	2.830	539	541	543	rBV	202	122	0.01%	0.002%
11	2.965	581	583	584	rBV	157	63	0.01%	0.001%
12	3.084	618	620	623	rBV	192	98	0.01%	0.001%
13	3.187	650	652	654	rBV	126	58	0.01%	0.001%
14	3.270	676	678	679	rBV	262	135	0.01%	0.002%
15	3.405	717	720	723	rBV2	259	242	0.03%	0.003%
16	3.470	737	740	743	rVB	276	163	0.02%	0.002%
17	3.492	743	747	748	rBV	266	164	0.02%	0.002%
18	3.717	812	817	819	rBV	282	238	0.03%	0.003%
19	3.746	824	826	829	rVV	206	108	0.01%	0.001%
20	3.785	834	838	840	rVV	164	151	0.02%	0.002%
21	3.868	862	864	865	rBV	63	29	0.00%	0.000%
22	3.907	865	876	916	rBV	64387	192124	20.75%	2.599%
23	4.373	1006	1021	1047	rBV	150215	372291	40.21%	5.036%
24	4.573	1078	1083	1084	rBV	334	225	0.02%	0.003%
25	4.637	1101	1103	1104	rBV	190	105	0.01%	0.001%
26	4.679	1113	1116	1121	rVB3	306	271	0.03%	0.004%
27	4.698	1121	1122	1124	rBV	227	94	0.01%	0.001%
28	4.756	1138	1140	1144	rVB2	337	203	0.02%	0.003%
29	4.775	1144	1146	1148	rBV	389	227	0.02%	0.003%
30	4.833	1158	1164	1166	rBV2	397	448	0.05%	0.006%
31	4.875	1175	1177	1180	rBV	226	147	0.02%	0.002%
32	4.897	1181	1184	1191	rVV2	218	241	0.03%	0.003%
33	4.978	1203	1209	1211	rBV2	289	272	0.03%	0.004%
34	5.071	1221	1238	1266	rBV2	359163	925903	100.00%	12.524%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102920\
 Data File : VV019168.D
 Acq On : 30 Oct 2020 00:45
 Operator : SY/MD
 Sample : L4502-18ME 40X
 Misc : 6.04g/5.0ml/100uL/5.0ml/MSVOA-V/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG441ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

35	5.364	1327	1329	1331	rBV	215	144	0.02%	0.002%
36	5.428	1346	1349	1352	rVB	319	214	0.02%	0.003%
37	5.463	1357	1360	1362	rBV2	309	240	0.03%	0.003%
38	5.515	1374	1376	1377	rBV2	132	53	0.01%	0.001%
39	5.579	1392	1396	1400	rVB2	251	227	0.02%	0.003%
40	5.640	1400	1415	1442	rBV	296809	584338	63.11%	7.904%
41	5.884	1489	1491	1492	rBV2	164	91	0.01%	0.001%
42	5.933	1497	1506	1520	rVB7	5388	11918	1.29%	0.161%
43	6.036	1536	1538	1539	rBV	150	60	0.01%	0.001%
44	6.093	1539	1556	1581	rBV	208351	416246	44.96%	5.630%
45	6.225	1595	1597	1600	rBV3	388	227	0.02%	0.003%
46	6.296	1618	1619	1620	rBV3	225	52	0.01%	0.001%
47	6.499	1678	1682	1684	rBV2	229	223	0.02%	0.003%
48	6.569	1701	1704	1708	rBV2	248	232	0.03%	0.003%
49	6.627	1717	1722	1724	rBV2	306	246	0.03%	0.003%
50	6.913	1808	1811	1819	rBV2	313	341	0.04%	0.005%
51	7.007	1829	1840	1867	rBV	117578	214563	23.17%	2.902%
52	7.241	1909	1913	1915	rBV	265	257	0.03%	0.003%
53	7.338	1931	1943	1961	rBV	424820	730432	78.89%	9.880%
54	7.540	2003	2006	2007	rBV2	455	227	0.02%	0.003%
55	7.643	2027	2038	2068	rBV	84802	148920	16.08%	2.014%
56	7.788	2081	2083	2084	rBV	255	71	0.01%	0.001%
57	7.929	2124	2127	2129	rBV	279	202	0.02%	0.003%
58	7.997	2137	2148	2172	rVB	133095	221627	23.94%	2.998%
59	8.106	2172	2182	2214	rBV	230476	404057	43.64%	5.465%
60	8.447	2282	2288	2293	rBV3	561	771	0.08%	0.010%
61	8.605	2334	2337	2339	rBV	282	193	0.02%	0.003%
62	8.871	2409	2420	2455	rBV	454823	731499	79.00%	9.894%
63	9.042	2471	2473	2475	rVB	323	149	0.02%	0.002%
64	9.061	2475	2479	2482	rBV3	362	256	0.03%	0.003%
65	9.077	2482	2484	2487	rBV2	297	177	0.02%	0.002%
66	9.093	2487	2489	2492	rBV	309	206	0.02%	0.003%
67	9.170	2506	2513	2516	rBV2	461	606	0.07%	0.008%
68	9.222	2524	2529	2533	rVB2	367	317	0.03%	0.004%
69	9.370	2572	2575	2577	rBV	203	174	0.02%	0.002%
70	9.402	2582	2585	2588	rBV2	343	232	0.03%	0.003%
71	9.579	2637	2640	2645	rBV2	270	282	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102920\
 Data File : VV019168.D
 Acq On : 30 Oct 2020 00:45
 Operator : SY/MD
 Sample : L4502-18ME 40X
 Misc : 6.04g/5.0ml/100uL/5.0ml/MSVOA-V/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG441ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

72	9.675	2665	2670	2672	rBV2	294	250	0.03%	0.003%
73	9.775	2697	2701	2702	rBV	208	124	0.01%	0.002%
74	9.936	2747	2751	2756	rVB2	242	233	0.03%	0.003%
75	10.145	2812	2816	2821	rVB4	1075	1047	0.11%	0.014%
76	10.180	2824	2827	2828	rBV2	244	149	0.02%	0.002%
77	10.235	2833	2844	2866	rVB	266768	419048	45.26%	5.668%
78	10.762	3005	3008	3009	rBV	218	109	0.01%	0.001%
79	10.788	3014	3016	3017	rBV	189	64	0.01%	0.001%
80	11.084	3105	3108	3110	rBV2	200	139	0.02%	0.002%
81	11.270	3155	3166	3187	rBV	472090	714711	77.19%	9.667%
82	11.646	3271	3283	3304	rBV	458590	716437	77.38%	9.690%
83	11.797	3326	3330	3332	rBV	354	272	0.03%	0.004%
84	12.331	3493	3496	3499	rBV	233	129	0.01%	0.002%
85	12.502	3545	3549	3551	rBV2	332	242	0.03%	0.003%
86	12.633	3585	3590	3592	rBV2	250	241	0.03%	0.003%
87	13.775	3941	3945	3947	rBV2	418	328	0.04%	0.004%


Sum of corrected areas: 7393250

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102920\
Data File : VV019168.D
Acq On : 30 Oct 2020 00:45
Operator : SY/MD
Sample : L4502-18ME 40X
Misc : 6.04g/5.0ml/100uL/5.0ml/MSVOA-V/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG441ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

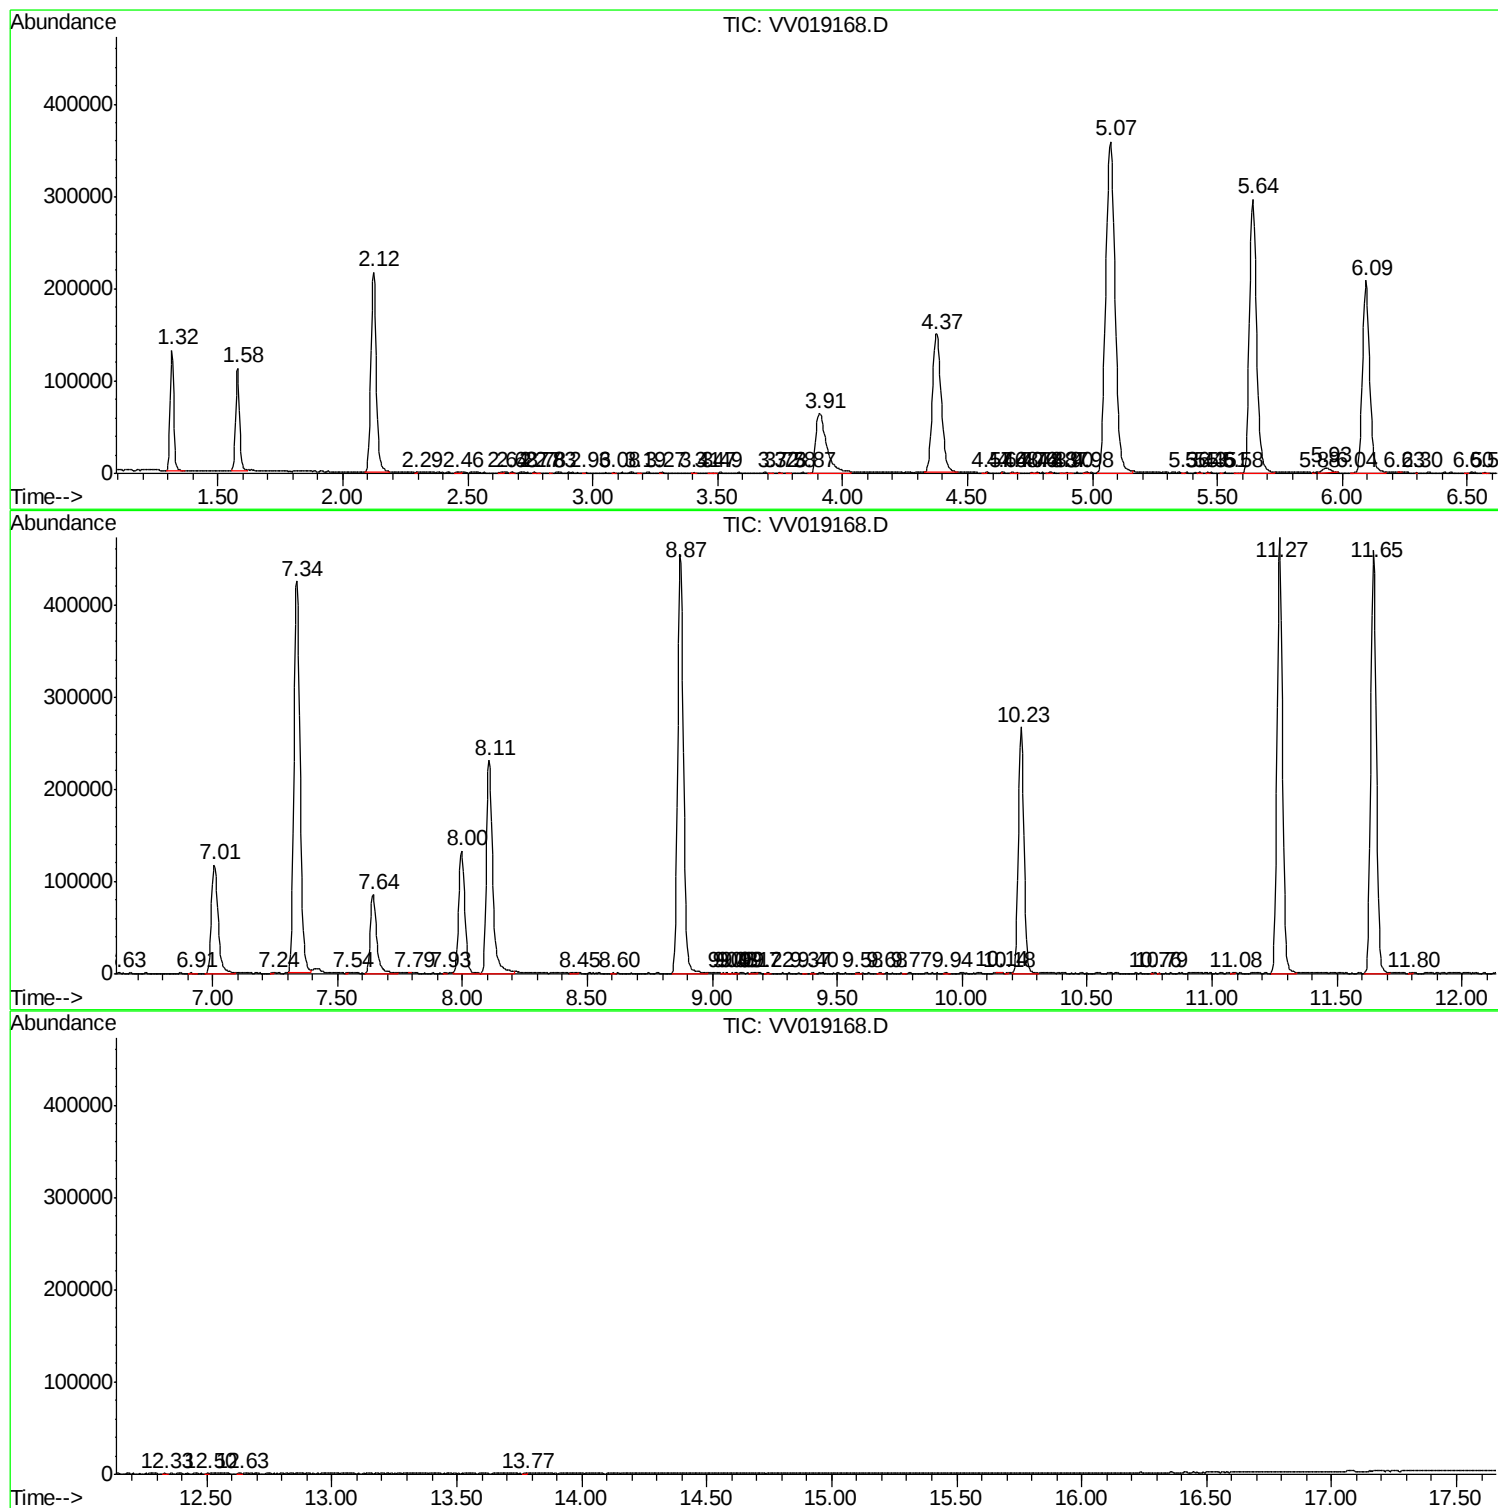

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102920\
Data File : VV019168.D
Acq On : 30 Oct 2020 00:45
Operator : SY/MD
Sample : L4502-18ME 40X
Misc : 6.04g/5.0ml/100uL/5.0ml/MSVOA-V/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG441ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV102920\
Data File : VV019168.D
Acq On : 30 Oct 2020 00:45
Operator : SY/MD
Sample : L4502-18ME 40X
Misc : 6.04g/5.0ml/100uL/5.0ml/MSV0A-V/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG441ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc