

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102920\
 Data File : VV019169.D
 Acq On : 30 Oct 2020 01:09
 Operator : SY/MD
 Sample : L4502-19ME 40X
 Misc : 6.01µl/5.0ml/100µl/5.0ml/MSVOA-V/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG442ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	85	rVB	133215	133981	13.99%	1.819%
2	1.579	145	152	164	rBV	109562	123563	12.90%	1.678%
3	2.123	310	321	344	rVB	217652	321941	33.62%	4.371%
4	2.389	399	404	406	rBV2	352	318	0.03%	0.004%
5	2.746	511	515	519	rBV	344	317	0.03%	0.004%
6	2.807	531	534	537	rBV2	289	170	0.02%	0.002%
7	2.888	555	559	564	rVV2	299	319	0.03%	0.004%
8	3.094	619	623	628	rBV	258	224	0.02%	0.003%
9	3.155	639	642	645	rBV2	229	181	0.02%	0.002%
10	3.290	680	684	686	rBV2	354	237	0.02%	0.003%
11	3.399	714	718	721	rBV2	193	164	0.02%	0.002%
12	3.441	729	731	736	rVB	262	166	0.02%	0.002%
13	3.531	756	759	762	rBV	312	216	0.02%	0.003%
14	3.605	779	782	785	rBV2	207	162	0.02%	0.002%
15	3.640	790	793	796	rVV2	312	220	0.02%	0.003%
16	3.679	803	805	810	rVB2	295	212	0.02%	0.003%
17	3.756	826	829	831	rBV	264	148	0.02%	0.002%
18	3.875	863	866	867	rBV	376	219	0.02%	0.003%
19	3.913	867	878	912	rBV3	67849	206288	21.54%	2.801%
20	4.376	1005	1022	1049	rBV	160125	388376	40.55%	5.273%
21	4.605	1090	1093	1097	rBV2	236	175	0.02%	0.002%
22	4.634	1101	1102	1106	rVB2	232	144	0.02%	0.002%
23	4.733	1131	1133	1139	rVB2	381	307	0.03%	0.004%
24	4.769	1139	1144	1148	rBV2	366	432	0.05%	0.006%
25	4.804	1153	1155	1159	rVV2	276	186	0.02%	0.003%
26	4.833	1161	1164	1168	rVB	238	147	0.02%	0.002%
27	4.913	1186	1189	1192	rBV2	160	141	0.01%	0.002%
28	4.952	1199	1201	1203	rBV2	367	229	0.02%	0.003%
29	5.071	1221	1238	1276	rVV2	371208	957703	100.00%	13.004%
30	5.399	1337	1340	1344	rVB2	251	171	0.02%	0.002%
31	5.425	1344	1348	1351	rBV2	239	258	0.03%	0.004%
32	5.466	1360	1361	1367	rVB	314	188	0.02%	0.003%
33	5.511	1372	1375	1378	rBV	280	212	0.02%	0.003%
34	5.640	1403	1415	1439	rBV	275250	545586	56.97%	7.408%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102920\
 Data File : VV019169.D
 Acq On : 30 Oct 2020 01:09
 Operator : SY/MD
 Sample : L4502-19ME 40X
 Misc : 6.01g/5.0ml/100uL/5.0ml/MSVOA-V/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG442ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

35	5.936	1496	1507	1523	rVB7	6131	12401	1.29%	0.168%
36	6.093	1542	1556	1587	rBV	212456	430120	44.91%	5.840%
37	6.502	1680	1683	1686	rBV2	228	142	0.01%	0.002%
38	6.576	1703	1706	1713	rBV2	282	396	0.04%	0.005%
39	6.659	1729	1732	1734	rBV	185	143	0.01%	0.002%
40	6.695	1741	1743	1746	rBV	190	144	0.02%	0.002%
41	6.769	1763	1766	1770	rBV2	198	170	0.02%	0.002%
42	6.814	1776	1780	1783	rBV	178	166	0.02%	0.002%
43	6.904	1802	1808	1809	rBV	258	245	0.03%	0.003%
44	7.007	1826	1840	1863	rBV	123435	220608	23.04%	2.995%
45	7.183	1890	1895	1898	rBV2	372	342	0.04%	0.005%
46	7.270	1919	1922	1926	rVB3	259	186	0.02%	0.003%
47	7.338	1930	1943	1962	rBV	432324	735429	76.79%	9.986%
48	7.640	2028	2037	2065	rBV	88448	153707	16.05%	2.087%
49	7.820	2090	2093	2102	rVB2	341	434	0.05%	0.006%
50	7.997	2136	2148	2169	rBV	136571	227928	23.80%	3.095%
51	8.106	2172	2182	2218	rBV	247191	425899	44.47%	5.783%
52	8.380	2264	2267	2268	rBV	302	162	0.02%	0.002%
53	8.492	2301	2302	2309	rVB2	332	214	0.02%	0.003%
54	8.524	2309	2312	2315	rVB2	251	162	0.02%	0.002%
55	8.547	2315	2319	2321	rBV	231	181	0.02%	0.002%
56	8.611	2337	2339	2343	rBV	211	148	0.02%	0.002%
57	8.669	2355	2357	2363	rBV	176	144	0.02%	0.002%
58	8.871	2408	2420	2446	rBV	416965	671002	70.06%	9.111%
59	9.080	2482	2485	2487	rBV2	186	137	0.01%	0.002%
60	9.170	2508	2513	2515	rBV3	434	363	0.04%	0.005%
61	9.251	2536	2538	2542	rVB	344	161	0.02%	0.002%
62	9.293	2548	2551	2555	rVB2	297	175	0.02%	0.002%
63	9.357	2565	2571	2572	rBV	236	245	0.03%	0.003%
64	9.431	2591	2594	2596	rBV2	222	152	0.02%	0.002%
65	9.656	2660	2664	2672	rBV2	354	398	0.04%	0.005%
66	9.691	2672	2675	2676	rBV	231	138	0.01%	0.002%
67	9.865	2727	2729	2733	rVB	307	170	0.02%	0.002%
68	9.887	2733	2736	2741	rBV2	290	229	0.02%	0.003%
69	9.926	2746	2748	2751	rBV	227	158	0.02%	0.002%
70	9.984	2762	2766	2769	rBV2	306	312	0.03%	0.004%
71	10.023	2775	2778	2781	rBV	227	164	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102920\
 Data File : VV019169.D
 Acq On : 30 Oct 2020 01:09
 Operator : SY/MD
 Sample : L4502-19ME 40X
 Misc : 6.01g/5.0ml/100uL/5.0ml/MSVOA-V/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG442ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

72	10.074	2790	2794	2796	rBV	200	142	0.01%	0.002%
73	10.145	2813	2816	2823	rVB5	1227	1234	0.13%	0.017%
74	10.235	2833	2844	2869	rVB	279833	438166	45.75%	5.950%
75	10.341	2875	2877	2879	rBV2	347	194	0.02%	0.003%
76	10.379	2884	2889	2892	rBV2	295	339	0.04%	0.005%
77	10.434	2902	2906	2910	rVB2	281	255	0.03%	0.003%
78	10.685	2980	2984	2987	rVB	254	179	0.02%	0.002%
79	10.707	2987	2991	2993	rBV2	280	189	0.02%	0.003%
80	10.759	3005	3007	3015	rVB	371	352	0.04%	0.005%
81	10.939	3058	3063	3064	rBV2	663	618	0.06%	0.008%
82	11.032	3089	3092	3096	rBV2	301	283	0.03%	0.004%
83	11.090	3105	3110	3116	rVB2	366	325	0.03%	0.004%
84	11.161	3129	3132	3136	rBV2	379	293	0.03%	0.004%
85	11.270	3155	3166	3193	rBV	421351	642150	67.05%	8.719%
86	11.447	3217	3221	3225	rBV2	668	626	0.07%	0.009%
87	11.540	3247	3250	3254	rBV2	284	235	0.02%	0.003%
88	11.646	3271	3283	3304	rBV	456179	709635	74.10%	9.636%
89	11.810	3331	3334	3337	rVB2	379	262	0.03%	0.004%
90	11.948	3372	3377	3381	rBV2	308	326	0.03%	0.004%
91	12.350	3496	3502	3507	rVB2	231	272	0.03%	0.004%
92	12.457	3532	3535	3538	rBV2	240	146	0.02%	0.002%
93	12.749	3624	3626	3628	rBV	243	168	0.02%	0.002%
94	12.929	3678	3682	3685	rBV	330	264	0.03%	0.004%
95	13.010	3705	3707	3710	rBV	292	219	0.02%	0.003%
96	13.251	3780	3782	3785	rBV2	260	207	0.02%	0.003%
97	13.421	3830	3835	3836	rBV	253	195	0.02%	0.003%
98	13.524	3865	3867	3872	rBV2	283	251	0.03%	0.003%
99	13.752	3935	3938	3943	rBV	299	260	0.03%	0.004%
100	14.505	4167	4172	4174	rBV	359	328	0.03%	0.004%


Sum of corrected areas: 7364689

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102920\
Data File : VV019169.D
Acq On : 30 Oct 2020 01:09
Operator : SY/MD
Sample : L4502-19ME 40X
Misc : 6.01a/5.0ml/100uL/5.0ml/MSVOA-V/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG442ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

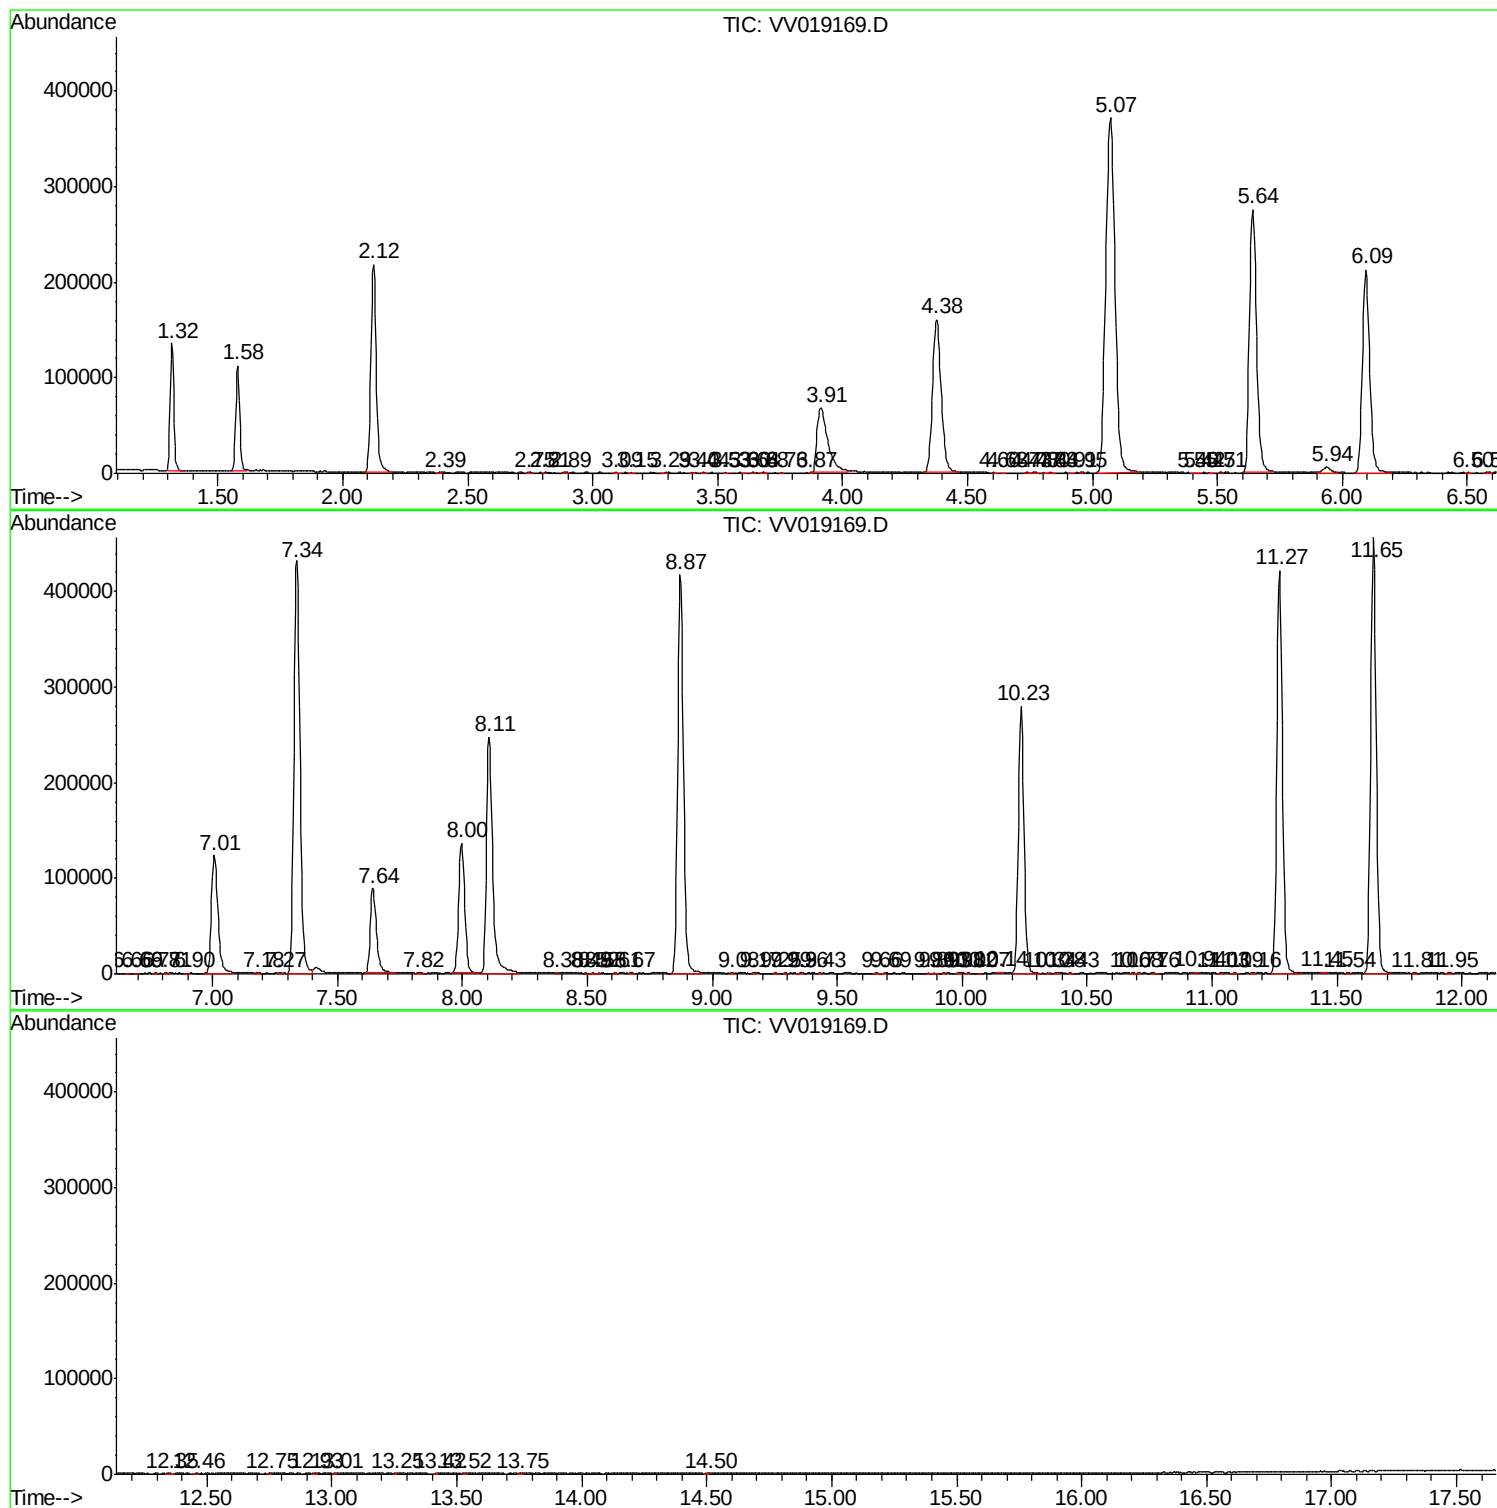

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102920\
Data File : VV019169.D
Acq On : 30 Oct 2020 01:09
Operator : SY/MD
Sample : L4502-19ME 40X
Misc : 6.01g/5.0ml/100uL/5.0ml/MSVOA-V/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG442ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV102920\
Data File : VV019169.D
Acq On : 30 Oct 2020 01:09
Operator : SY/MD
Sample : L4502-19ME 40X
Misc : 6.01g/5.0ml/100uL/5.0ml/MSV0A-V/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG442ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc