

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102920\
 Data File : VV019170.D
 Acq On : 30 Oct 2020 01:33
 Operator : SY/MD
 Sample : L4502-20ME 4X
 Misc : 6.07g/5.0ml/100uL/5.0ml/MSVOA-V/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG443ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	83	rVB	137810	138415	14.21%	1.751%
2	1.576	144	151	161	rBV	115254	131979	13.55%	1.670%
3	2.116	309	319	348	rVB	232128	344946	35.42%	4.364%
4	2.261	362	364	366	rBV	386	163	0.02%	0.002%
5	2.521	437	445	452	rBV4	1254	1749	0.18%	0.022%
6	2.579	461	463	465	rBV	171	105	0.01%	0.001%
7	2.634	468	480	496	rVV2	6007	13648	1.40%	0.173%
8	2.958	577	581	584	rBV	276	238	0.02%	0.003%
9	3.016	596	599	602	rBV2	205	168	0.02%	0.002%
10	3.077	615	618	621	rBV2	195	152	0.02%	0.002%
11	3.151	639	641	646	rVB2	333	260	0.03%	0.003%
12	3.180	646	650	654	rBV2	268	273	0.03%	0.003%
13	3.222	660	663	667	rVB	341	273	0.03%	0.003%
14	3.283	678	682	685	rVB2	322	268	0.03%	0.003%
15	3.306	685	689	693	rBV2	194	166	0.02%	0.002%
16	3.325	693	695	697	rBV	169	100	0.01%	0.001%
17	3.357	702	705	706	rBV	261	131	0.01%	0.002%
18	3.389	713	715	717	rBV	222	106	0.01%	0.001%
19	3.431	725	728	730	rBV2	258	173	0.02%	0.002%
20	3.463	735	738	743	rVB2	232	172	0.02%	0.002%
21	3.486	743	745	750	rBV	152	110	0.01%	0.001%
22	3.515	751	754	756	rBV	168	121	0.01%	0.002%
23	3.585	771	776	779	rVB2	260	217	0.02%	0.003%
24	3.614	779	785	787	rBV	254	276	0.03%	0.003%
25	3.663	797	800	804	rVB	370	247	0.03%	0.003%
26	3.698	804	811	816	rBV	288	332	0.03%	0.004%
27	3.720	816	818	821	rBV	148	93	0.01%	0.001%
28	3.910	867	877	913	rBV	61595	193738	19.90%	2.451%
29	4.264	985	987	991	rBV2	332	215	0.02%	0.003%
30	4.373	1004	1021	1048	rBV	160679	390416	40.09%	4.939%
31	4.518	1064	1066	1071	rVB2	535	360	0.04%	0.005%
32	4.544	1071	1074	1077	rVB	274	150	0.02%	0.002%
33	4.563	1077	1080	1082	rBV	305	171	0.02%	0.002%
34	4.592	1086	1089	1092	rBV2	229	135	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102920\
 Data File : VV019170.D
 Acq On : 30 Oct 2020 01:33
 Operator : SY/MD
 Sample : L4502-20ME 4X
 Misc : 6.07g/5.0ml/100uL/5.0ml/MSVOA-V/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG443ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

35	4.611	1092	1095	1099	rBV3	370	290	0.03%	0.004%
36	4.691	1117	1120	1124	rBV2	218	208	0.02%	0.003%
37	4.884	1176	1180	1182	rBV2	113	93	0.01%	0.001%
38	4.936	1192	1196	1199	rBV	250	194	0.02%	0.002%
39	5.068	1220	1237	1271	rBV2	385287	973767	100.00%	12.319%
40	5.495	1368	1370	1373	rBV2	231	171	0.02%	0.002%
41	5.588	1396	1399	1402	rBV	315	280	0.03%	0.004%
42	5.640	1403	1415	1439	rBV2	287733	572384	58.78%	7.241%
43	5.939	1493	1508	1522	rBV8	7381	17464	1.79%	0.221%
44	6.010	1522	1530	1531	rBV2	464	454	0.05%	0.006%
45	6.090	1543	1555	1584	rBV	213318	431685	44.33%	5.461%
46	6.289	1614	1617	1621	rVB	460	280	0.03%	0.004%
47	6.859	1790	1794	1797	rBV2	216	208	0.02%	0.003%
48	6.916	1809	1812	1814	rBV2	248	166	0.02%	0.002%
49	7.006	1828	1840	1866	rBV	123119	223641	22.97%	2.829%
50	7.199	1897	1900	1903	rBV2	335	250	0.03%	0.003%
51	7.338	1928	1943	1961	rBV	458458	790941	81.22%	10.006%
52	7.640	2027	2037	2061	rBV2	90921	156503	16.07%	1.980%
53	7.997	2135	2148	2170	rBV	228009	381846	39.21%	4.831%
54	8.109	2173	2183	2221	rBV	209612	434782	44.65%	5.500%
55	8.302	2240	2243	2245	rBV2	380	257	0.03%	0.003%
56	8.386	2266	2269	2271	rBV	448	313	0.03%	0.004%
57	8.440	2281	2286	2293	rBV3	1142	1474	0.15%	0.019%
58	8.492	2299	2302	2305	rBV2	250	142	0.01%	0.002%
59	8.598	2332	2335	2337	rBV	272	184	0.02%	0.002%
60	8.666	2353	2356	2360	rVB2	317	271	0.03%	0.003%
61	8.788	2391	2394	2396	rBV2	187	119	0.01%	0.002%
62	8.871	2409	2420	2447	rBV	441935	716554	73.59%	9.065%
63	9.112	2491	2495	2499	rBV2	283	305	0.03%	0.004%
64	9.228	2528	2531	2533	rBV2	232	149	0.02%	0.002%
65	9.428	2588	2593	2599	rVB2	347	434	0.04%	0.005%
66	9.457	2599	2602	2606	rBV	188	148	0.02%	0.002%
67	9.620	2649	2653	2656	rBV	318	259	0.03%	0.003%
68	9.662	2660	2666	2668	rBV2	303	320	0.03%	0.004%
69	9.727	2684	2686	2688	rBV	238	116	0.01%	0.001%
70	9.797	2705	2708	2713	rVB	374	289	0.03%	0.004%
71	9.820	2713	2715	2719	rBV	165	119	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102920\
 Data File : VV019170.D
 Acq On : 30 Oct 2020 01:33
 Operator : SY/MD
 Sample : L4502-20ME 4X
 Misc : 6.07g/5.0ml/100uL/5.0ml/MSVOA-V/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG443ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

72	9.926	2744	2748	2751	rBV	211	209	0.02%	0.003%
73	9.945	2751	2754	2758	rVB	333	225	0.02%	0.003%
74	9.968	2758	2761	2763	rBV	308	188	0.02%	0.002%
75	10.058	2781	2789	2793	rBV	411	624	0.06%	0.008%
76	10.151	2812	2818	2823	rVB3	1283	1451	0.15%	0.018%
77	10.238	2833	2845	2863	rBV	279027	443053	45.50%	5.605%
78	10.485	2920	2922	2924	rBV3	285	172	0.02%	0.002%
79	10.521	2931	2933	2936	rBV	181	118	0.01%	0.001%
80	10.817	3020	3025	3026	rBV2	362	309	0.03%	0.004%
81	10.936	3055	3062	3072	rBV5	1295	2125	0.22%	0.027%
82	11.161	3128	3132	3140	rBV4	565	630	0.06%	0.008%
83	11.219	3148	3150	3153	rVB	302	148	0.02%	0.002%
84	11.270	3153	3166	3185	rBV	482667	734331	75.41%	9.290%
85	11.514	3238	3242	3247	rBV	265	321	0.03%	0.004%
86	11.569	3255	3259	3262	rBV2	322	356	0.04%	0.005%
87	11.646	3271	3283	3307	rBV	511456	789762	81.10%	9.991%
88	11.765	3317	3320	3326	rVB2	481	555	0.06%	0.007%
89	11.797	3326	3330	3331	rBV2	231	145	0.01%	0.002%
90	11.836	3335	3342	3348	rBV2	346	532	0.05%	0.007%
91	11.865	3350	3351	3354	rBV	207	100	0.01%	0.001%
92	12.042	3404	3406	3408	rBV	223	84	0.01%	0.001%
93	12.135	3433	3435	3437	rBV	185	92	0.01%	0.001%
94	12.148	3437	3439	3443	rVB	296	165	0.02%	0.002%
95	12.778	3633	3635	3637	rBV2	278	111	0.01%	0.001%
96	13.151	3748	3751	3758	rBV2	276	364	0.04%	0.005%
97	13.260	3780	3785	3790	rVB2	408	383	0.04%	0.005%
98	13.540	3869	3872	3875	rBV2	265	244	0.03%	0.003%
99	13.585	3883	3886	3890	rBV2	220	213	0.02%	0.003%
100	13.633	3897	3901	3907	rBV	450	476	0.05%	0.006%


Sum of corrected areas: 7904612

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102920\
Data File : VV019170.D
Acq On : 30 Oct 2020 01:33
Operator : SY/MD
Sample : L4502-20ME 4X
Misc : 6.07g/5.0ml/100uL/5.0ml/MSVOA-V/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG443ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

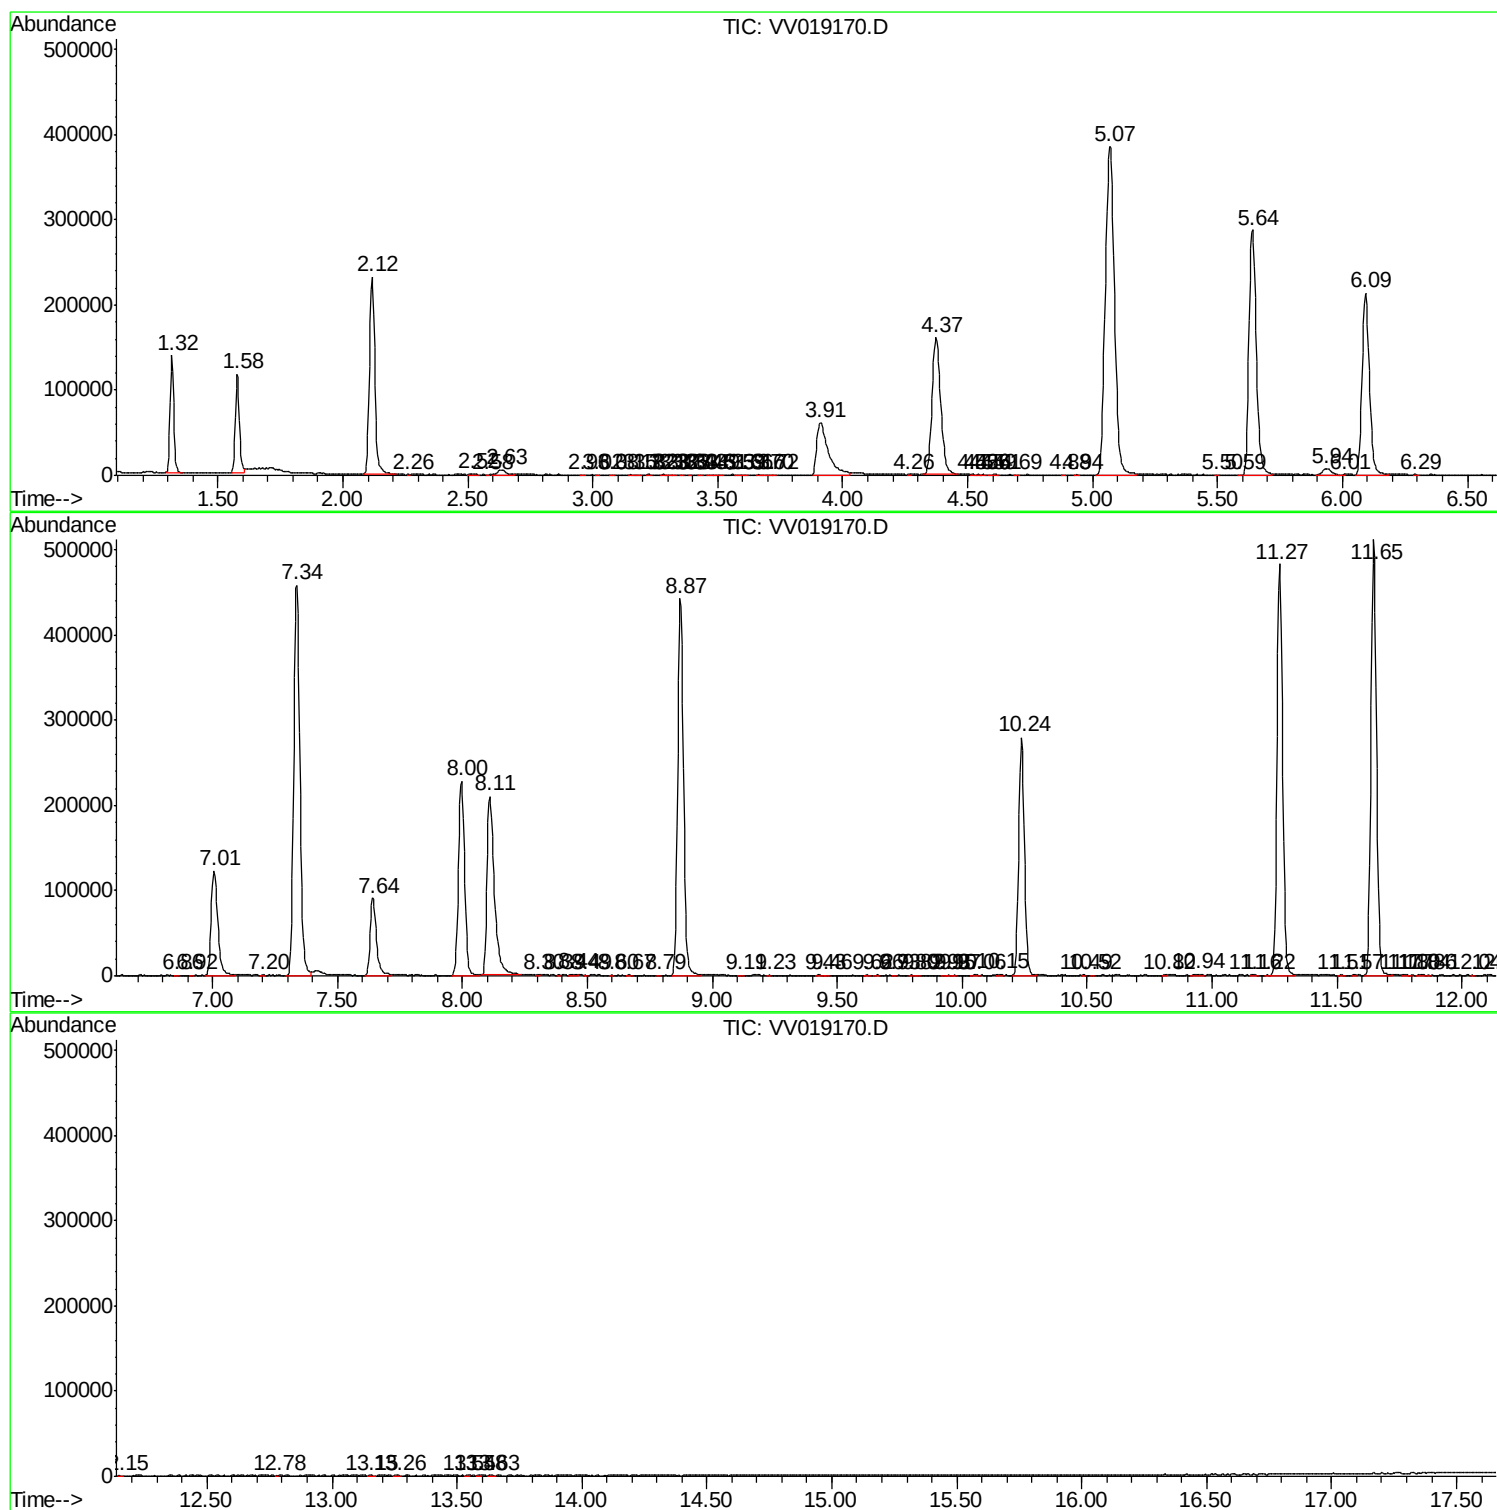

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102920\
Data File : VV019170.D
Acq On : 30 Oct 2020 01:33
Operator : SY/MD
Sample : L4502-20ME 4X
Misc : 6.07g/5.0ml/100uL/5.0ml/MSVOA-V/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG443ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV102920\
Data File : VV019170.D
Acq On : 30 Oct 2020 01:33
Operator : SY/MD
Sample : L4502-20ME 4X
Misc : 6.07g/5.0ml/100uL/5.0ml/MSV0A-V/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG443ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
