


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV102920\
 Data File : VV019144.D
 Acq On : 29 Oct 2020 12:34
 Operator : SY/MD
 Sample : BFB85
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB85

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis
 Last Update : Fri Oct 30 05:31:22 2020

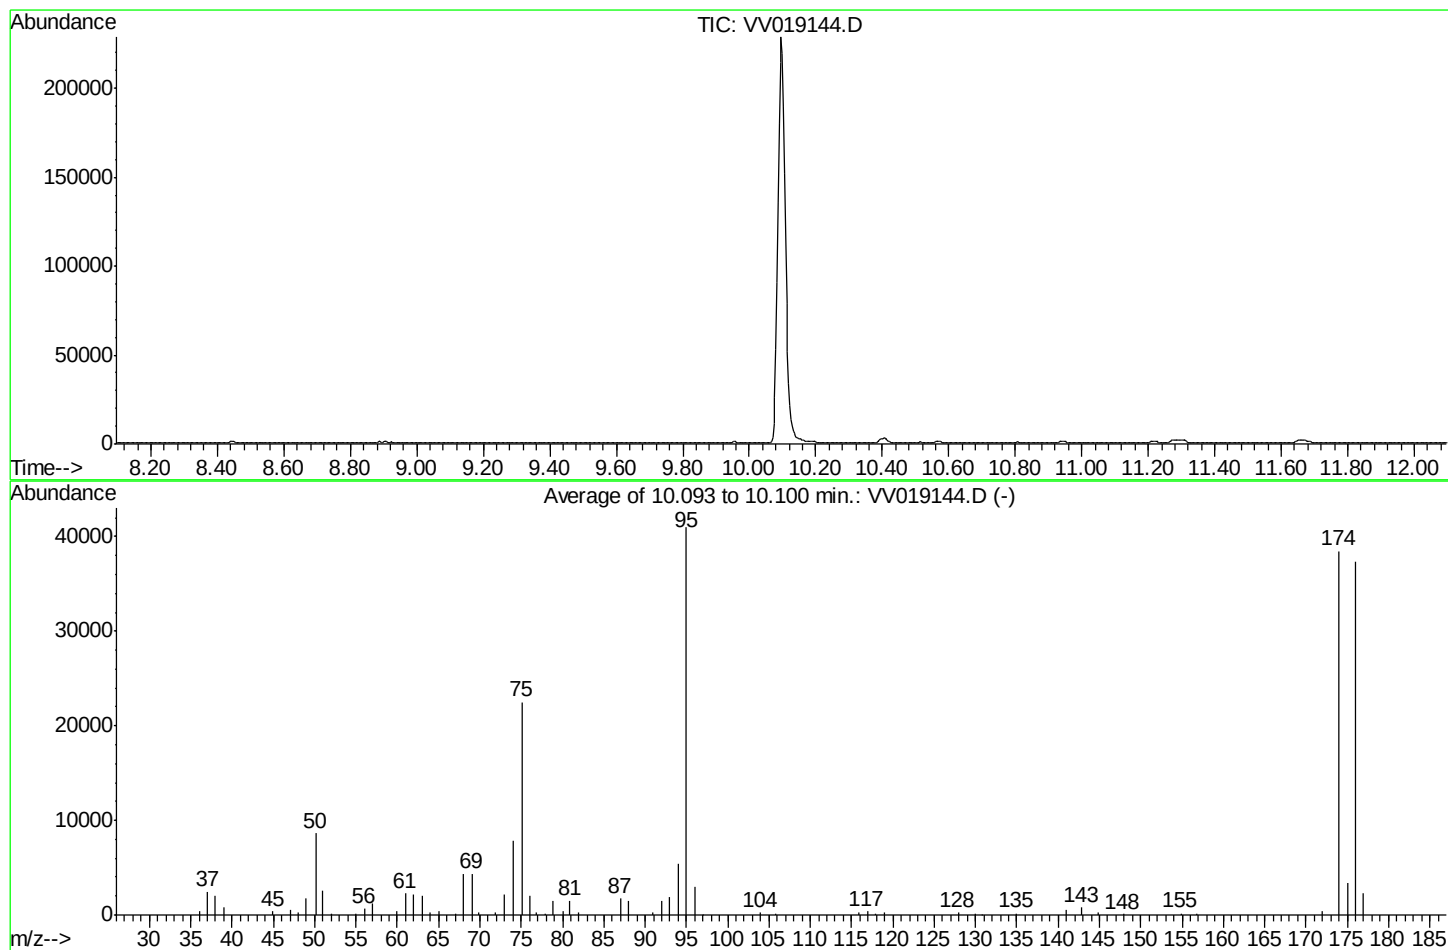

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	8596	PASS
75	95	30	80	55.0	22525	PASS
95	95	100	100	100.0	40973	PASS
96	95	5	9	7.2	2954	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	93.8	38450	PASS
175	174	5	9	8.8	3377	PASS
176	174	95	101	97.3	37408	PASS
177	176	5	9	6.3	2367	PASS

m/z	Abundance
36.00	394.0
37.00	2400.0
38.00	1941.0
39.00	812.0
40.00	110.0
44.00	835.0
44.90	379.0
47.00	495.0
47.90	314.0
49.00	1726.0
50.10	8498.0
51.00	2516.0
52.00	150.0
54.90	152.0
56.10	640.0
57.00	1293.0
60.00	469.0
61.00	2272.0
62.00	2133.0
63.00	2193.0
63.90	306.0
65.00	285.0
67.10	161.0
68.00	4279.0
69.00	4325.0
69.90	299.0
71.90	276.0
73.00	2167.0
74.00	7747.0
75.10	22176.0
76.00	2153.0
76.90	212.0
78.00	209.0
78.90	1416.0
80.00	469.0
80.90	1464.0
81.90	278.0
87.00	1667.0
87.90	1428.0
90.90	241.0
92.00	1335.0
93.00	1875.0
94.10	5261.0
95.00	39808.0
96.00	2948.0
96.90	101.0
103.90	200.0
105.90	185.0
115.90	259.0
116.90	343.0
117.80	189.0
118.90	308.0
127.90	206.0
129.90	111.0
130.70	104.0
134.90	149.0
140.90	568.0
142.90	741.0
144.80	224.0
147.90	117.0
154.90	156.0
156.80	116.0
171.90	427.0
174.00	36704.0
175.00	3265.0
176.00	35328.0
177.00	2314.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

m/z	Abundance
36.00	461.0
37.00	2600.0
38.00	2100.0
39.00	758.0
40.00	117.0
44.00	828.0
44.90	383.0
47.00	542.0
48.00	319.0
49.00	1829.0
50.10	8904.0
51.00	2661.0
52.00	149.0
54.90	146.0
56.00	693.0
57.00	1337.0
60.00	443.0
61.00	2323.0
62.00	2276.0
63.00	2172.0
63.90	312.0
65.00	350.0
67.10	133.0
68.00	4425.0
69.00	4490.0
69.90	346.0
71.90	254.0
73.00	2304.0
74.00	8091.0
75.10	23344.0
76.00	2147.0
76.90	224.0
77.90	203.0
78.90	1508.0
80.00	479.0
80.90	1597.0
81.90	285.0
87.00	1830.0
87.90	1503.0
90.90	316.0
92.00	1538.0
93.00	2029.0
94.00	5563.0
95.00	42400.0
96.00	3088.0
104.00	230.0
105.80	185.0
115.90	231.0
116.90	396.0
117.80	208.0
118.90	331.0
128.00	227.0
129.90	122.0
130.70	107.0
134.90	168.0
140.90	525.0
142.90	791.0
144.80	225.0
147.90	133.0
154.80	219.0
156.80	132.0
172.00	401.0
174.00	39768.0
175.00	3523.0
176.00	38792.0
177.00	2458.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

m/z	Abundance
36.00	463.0
37.10	2387.0
38.00	1997.0
39.00	695.0
40.00	117.0
44.00	790.0
45.00	374.0
47.10	494.0
48.00	289.0
49.00	1776.0
50.10	8387.0
51.00	2642.0
52.00	114.0
55.00	148.0
56.00	682.0
57.10	1180.0
60.00	445.0
61.00	2236.0
62.00	2173.0
63.10	1897.0
63.90	280.0
65.00	438.0
66.90	120.0
68.00	4307.0
69.00	4245.0
69.90	352.0
71.90	241.0
73.00	2060.0
74.00	7558.0
75.10	22056.0
76.00	1830.0
76.80	236.0
77.90	156.0
78.90	1456.0
80.00	433.0
80.90	1526.0
81.90	299.0
87.00	1723.0
88.00	1454.0
90.90	326.0
92.00	1533.0
93.00	1908.0
94.00	5269.0
95.00	40712.0
96.00	2826.0
103.90	197.0
105.80	185.0
115.90	176.0
116.90	404.0
117.90	218.0
118.90	316.0
127.90	192.0
129.90	135.0
135.00	166.0
140.90	479.0
142.90	733.0
144.80	179.0
147.90	113.0
154.80	246.0
156.80	110.0
172.00	341.0
174.00	38880.0
175.00	3343.0
176.00	38104.0
177.00	2331.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

Scan 2790 (10.061 min): VV019144.D
BFB85

m/z	Abundance
39.90	146.0
44.00	850.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85