

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102921\
 Data File : VV023093.D
 Acq On : 29 Oct 2021 10:24
 Operator : SY/MD
 Sample : VV1029MBL03
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK268

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
 Title : VOC Analysis

Signal : TIC: VV023093.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	96	rVB	147775	152364	13.67%	1.815%
2	1.564	157	163	179	rVB	123843	140122	12.57%	1.669%
3	2.108	321	332	359	rVB	251980	376856	33.82%	4.488%
4	2.494	450	452	453	rBV2	976	444	0.04%	0.005%
5	2.555	468	471	473	rBV2	434	229	0.02%	0.003%
6	2.625	489	493	496	rBV2	411	389	0.03%	0.005%
7	2.664	503	505	509	rVB3	518	333	0.03%	0.004%
8	2.693	511	514	515	rBV2	437	190	0.02%	0.002%
9	2.728	521	525	526	rBV	425	298	0.03%	0.004%
10	3.008	608	612	615	rBV	388	264	0.02%	0.003%
11	3.082	631	635	640	rBV3	255	197	0.02%	0.002%
12	3.259	685	690	691	rBV2	438	292	0.03%	0.003%
13	3.667	815	817	821	rBV2	330	164	0.01%	0.002%
14	3.715	830	832	838	rVB2	251	206	0.02%	0.002%
15	3.799	854	858	860	rBB2	362	279	0.03%	0.003%
16	3.834	865	869	871	rBV2	412	253	0.02%	0.003%
17	3.873	871	881	917	rBV	83015	227744	20.44%	2.713%
18	4.262	1000	1002	1004	rBV2	473	176	0.02%	0.002%
19	4.346	1013	1028	1055	rVB	180726	447637	40.17%	5.332%
20	4.625	1110	1115	1118	rBV3	563	530	0.05%	0.006%
21	4.674	1128	1130	1134	rVB3	412	200	0.02%	0.002%
22	4.725	1142	1146	1149	rBV3	311	261	0.02%	0.003%
23	4.741	1149	1151	1154	rBV3	377	238	0.02%	0.003%
24	4.838	1175	1181	1183	rBV2	290	310	0.03%	0.004%
25	4.873	1190	1192	1197	rVB	487	260	0.02%	0.003%
26	5.043	1227	1245	1277	rBV2	433824	1114444	100.00%	13.273%
27	5.432	1364	1366	1369	rVB	618	252	0.02%	0.003%
28	5.471	1376	1378	1383	rVB4	521	276	0.02%	0.003%
29	5.538	1395	1399	1403	rBV3	343	395	0.04%	0.005%
30	5.612	1410	1422	1453	rBV	324280	652873	58.58%	7.776%
31	5.767	1468	1470	1472	rBV3	765	367	0.03%	0.004%
32	5.911	1505	1515	1527	rVB9	3687	8242	0.74%	0.098%
33	5.953	1527	1528	1531	rVB	492	190	0.02%	0.002%
34	6.066	1550	1563	1590	rBV	248055	510498	45.81%	6.080%
35	6.413	1669	1671	1673	rBV	276	175	0.02%	0.002%
36	6.506	1697	1700	1702	rBV3	309	240	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102921\
 Data File : VV023093.D
 Acq On : 29 Oct 2021 10:24
 Operator : SY/MD
 Sample : VV1029MBL03
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK268

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
 Title : VOC Analysis

37	6.529	1705	1707	1710	rVV2	416	202	0.02%	0.002%
38	6.545	1710	1712	1716	rVB4	555	261	0.02%	0.003%
39	6.622	1733	1736	1737	rBV2	658	330	0.03%	0.004%
40	6.693	1756	1758	1761	rVV	468	240	0.02%	0.003%
41	6.735	1768	1771	1773	rVB2	270	176	0.02%	0.002%
42	6.770	1779	1782	1785	rBV	244	152	0.01%	0.002%
43	6.982	1838	1848	1873	rBV	129372	243383	21.84%	2.899%
44	7.313	1938	1951	1970	rBV	509753	873771	78.40%	10.407%
45	7.561	2025	2028	2033	rVB2	388	282	0.03%	0.003%
46	7.583	2033	2035	2036	rBV	443	185	0.02%	0.002%
47	7.619	2036	2046	2065	rBV2	96880	168809	15.15%	2.011%
48	7.812	2103	2106	2108	rBV	315	216	0.02%	0.003%
49	7.937	2143	2145	2151	rBV3	459	266	0.02%	0.003%
50	7.972	2153	2156	2157	rBV2	312	172	0.02%	0.002%
51	7.979	2157	2158	2161	rVB2	715	298	0.03%	0.004%
52	7.995	2161	2163	2166	rVB2	424	154	0.01%	0.002%
53	8.085	2181	2191	2223	rBV	285866	496764	44.58%	5.917%
54	8.368	2277	2279	2283	rBV	404	219	0.02%	0.003%
55	8.484	2311	2315	2317	rBV	527	411	0.04%	0.005%
56	8.529	2327	2329	2332	rBV3	444	171	0.02%	0.002%
57	8.661	2368	2370	2372	rBV	308	162	0.01%	0.002%
58	8.728	2389	2391	2395	rVB2	436	188	0.02%	0.002%
59	8.850	2418	2429	2447	rBV	493104	792782	71.14%	9.442%
60	9.088	2501	2503	2506	rVB2	622	304	0.03%	0.004%
61	9.149	2516	2522	2527	rBV4	1232	1492	0.13%	0.018%
62	9.214	2537	2542	2547	rBV4	432	440	0.04%	0.005%
63	9.236	2547	2549	2551	rVB	365	180	0.02%	0.002%
64	9.352	2582	2585	2586	rBV2	578	274	0.02%	0.003%
65	9.451	2614	2616	2621	rVB2	359	231	0.02%	0.003%
66	9.580	2654	2656	2661	rVB5	616	352	0.03%	0.004%
67	9.705	2692	2695	2697	rBV	438	178	0.02%	0.002%
68	9.834	2731	2735	2737	rBV	204	160	0.01%	0.002%
69	9.979	2777	2780	2784	rBV2	224	180	0.02%	0.002%
70	10.127	2816	2826	2839	rBV4	3230	4917	0.44%	0.059%
71	10.217	2842	2854	2874	rBV	351635	548774	49.24%	6.536%
72	10.464	2928	2931	2932	rBV	508	262	0.02%	0.003%
73	10.538	2951	2954	2959	rBV3	444	460	0.04%	0.005%
74	10.596	2970	2972	2974	rBV2	480	293	0.03%	0.003%
75	10.860	3051	3054	3058	rBV4	321	256	0.02%	0.003%
76	10.914	3067	3071	3081	rVB6	2762	3823	0.34%	0.046%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102921\
 Data File : VV023093.D
 Acq On : 29 Oct 2021 10:24
 Operator : SY/MD
 Sample : VV1029MBL03
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK268

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
 Title : VOC Analysis

77	11.037	3103	3109	3114	rBV4	757	786	0.07%	0.009%
78	11.114	3131	3133	3135	rBV2	317	160	0.01%	0.002%
79	11.191	3151	3157	3164	rBV3	1272	1750	0.16%	0.021%
80	11.249	3164	3175	3194	rBV	507379	772776	69.34%	9.204%
81	11.477	3244	3246	3247	rBV2	384	155	0.01%	0.002%
82	11.625	3280	3292	3312	rBV	523934	819885	73.57%	9.765%
83	11.795	3337	3345	3352	rVB9	1268	1907	0.17%	0.023%
84	11.824	3352	3354	3355	rBV	394	167	0.01%	0.002%
85	12.085	3432	3435	3440	rBV2	729	628	0.06%	0.007%
86	12.162	3457	3459	3461	rBV	304	150	0.01%	0.002%
87	12.651	3607	3611	3621	rVB6	1440	1805	0.16%	0.021%
88	12.689	3621	3623	3626	rVB2	486	224	0.02%	0.003%
89	13.062	3736	3739	3742	rVB	317	181	0.02%	0.002%
90	13.114	3751	3755	3759	rBV2	280	259	0.02%	0.003%
91	13.139	3759	3763	3766	rVB2	474	345	0.03%	0.004%
92	13.265	3795	3802	3810	rVB9	2342	3602	0.32%	0.043%
93	13.297	3810	3812	3815	rBV2	283	176	0.02%	0.002%
94	13.371	3833	3835	3838	rBV3	468	213	0.02%	0.003%
95	13.406	3843	3846	3848	rBV3	432	286	0.03%	0.003%
96	13.509	3872	3878	3886	rVB3	3448	4739	0.43%	0.056%
97	13.750	3945	3953	3960	rBV6	2914	4438	0.40%	0.053%
98	13.998	4029	4030	4035	rVB2	489	299	0.03%	0.004%
99	14.027	4035	4039	4040	rBV2	488	305	0.03%	0.004%
100	14.155	4075	4079	4081	rBV3	689	463	0.04%	0.006%




Sum of corrected areas: 8396057

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102921\
Data File : VV023093.D
Acq On : 29 Oct 2021 10:24
Operator : SY/MD
Sample : VV1029MBL03
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK268

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

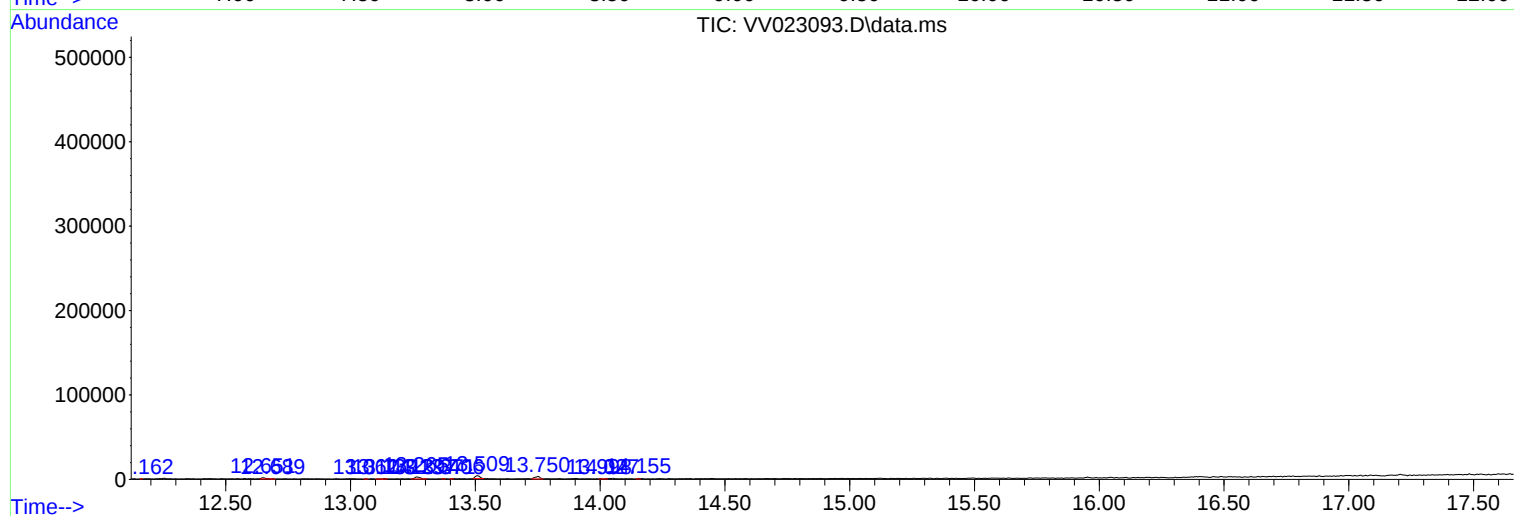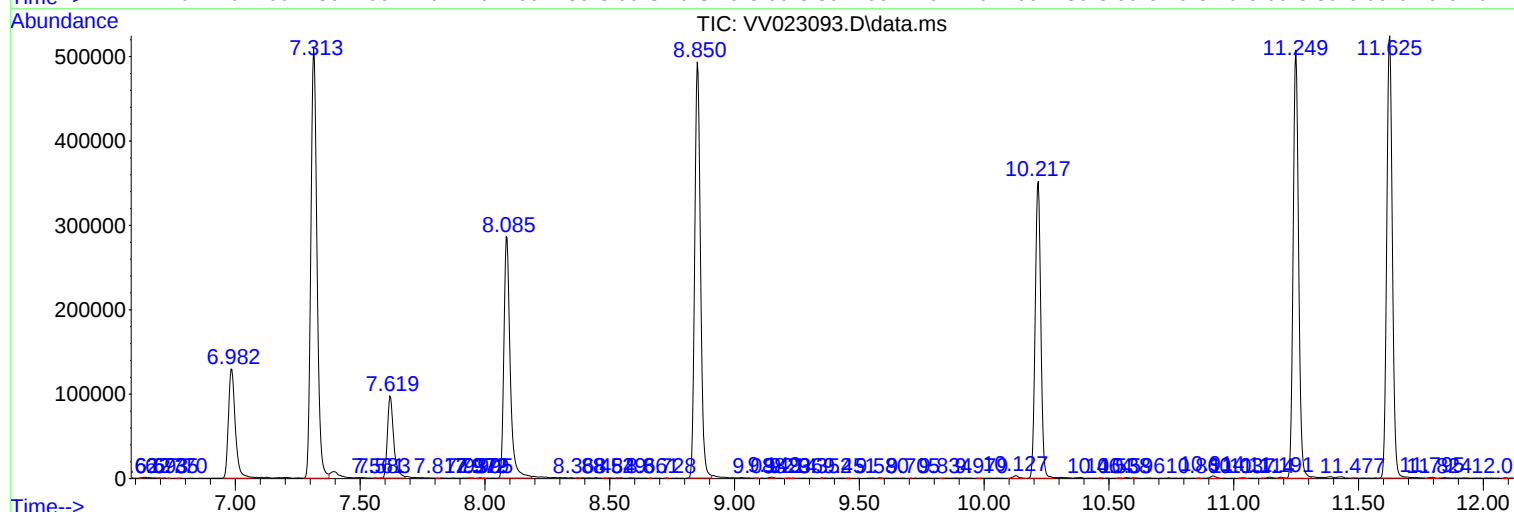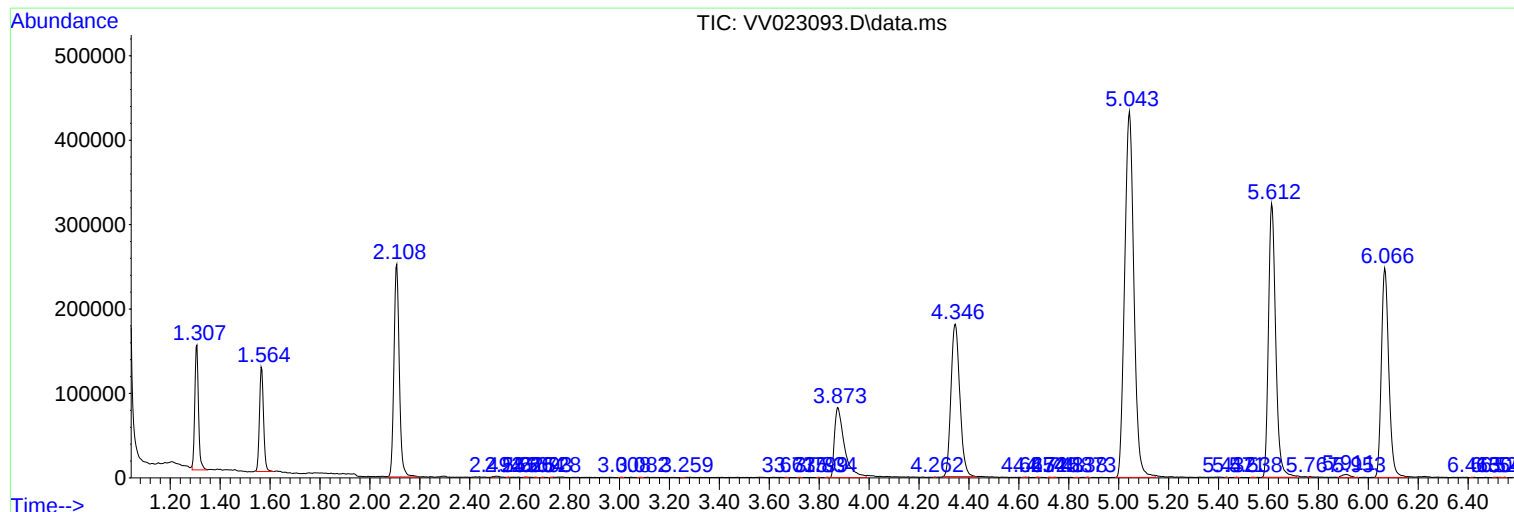

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102921\
Data File : VV023093.D
Acq On : 29 Oct 2021 10:24
Operator : SY/MD
Sample : VV1029MBL03
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK268

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102921\
Data File : VV023093.D
Acq On : 29 Oct 2021 10:24
Operator : SY/MD
Sample : VV1029MBL03
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK268

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
