

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102921\
 Data File : VV023095.D
 Acq On : 29 Oct 2021 11:12
 Operator : SY/MD
 Sample : VV1029MBL05
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK270

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M

Title : VOC Analysis

Signal : TIC: VV023095.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	98	rVB	143861	147883	13.48%	1.775%
2	1.568	157	164	176	rBV	118707	130309	11.88%	1.564%
3	2.108	321	332	352	rBV	253593	371599	33.87%	4.461%
4	2.217	364	366	370	rVB4	603	322	0.03%	0.004%
5	2.503	451	455	464	rVB6	1283	1867	0.17%	0.022%
6	2.661	499	504	507	rBV3	437	342	0.03%	0.004%
7	2.690	511	513	515	rVB3	414	163	0.01%	0.002%
8	2.719	520	522	527	rBV3	378	229	0.02%	0.003%
9	2.770	535	538	541	rVB2	585	349	0.03%	0.004%
10	2.790	542	544	549	rVB2	332	215	0.02%	0.003%
11	2.957	593	596	599	rVB2	501	284	0.03%	0.003%
12	3.169	660	662	663	rBV	287	139	0.01%	0.002%
13	3.237	680	683	685	rBV2	252	131	0.01%	0.002%
14	3.346	715	717	723	rVB3	425	267	0.02%	0.003%
15	3.407	734	736	739	rBV2	331	203	0.02%	0.002%
16	3.552	778	781	786	rBV3	344	288	0.03%	0.003%
17	3.664	814	816	820	rVB2	264	172	0.02%	0.002%
18	3.741	838	840	842	rBV	301	159	0.01%	0.002%
19	3.880	873	883	919	rBV2	85981	235999	21.51%	2.833%
20	4.153	966	968	969	rBV	606	233	0.02%	0.003%
21	4.285	1007	1009	1011	rBV2	526	173	0.02%	0.002%
22	4.349	1014	1029	1056	rVV2	180443	447561	40.80%	5.373%
23	4.622	1112	1114	1117	rBV	376	221	0.02%	0.003%
24	4.748	1147	1153	1157	rBV2	498	451	0.04%	0.005%
25	4.944	1211	1214	1219	rBV2	294	346	0.03%	0.004%
26	4.989	1224	1228	1229	rBV	371	184	0.02%	0.002%
27	5.047	1229	1246	1271	rBV2	424978	1097079	100.00%	13.171%
28	5.397	1349	1355	1356	rBV2	285	265	0.02%	0.003%
29	5.407	1356	1358	1360	rBV2	286	143	0.01%	0.002%
30	5.484	1374	1382	1383	rBV3	410	411	0.04%	0.005%
31	5.558	1403	1405	1407	rBV2	286	145	0.01%	0.002%
32	5.619	1411	1424	1447	rBV	316206	637628	58.12%	7.655%
33	5.838	1490	1492	1495	rVB3	628	334	0.03%	0.004%
34	5.915	1507	1516	1527	rVB8	3011	5869	0.53%	0.070%
35	6.069	1551	1564	1591	rBV	245325	506233	46.14%	6.078%
36	6.259	1619	1623	1624	rBV	417	346	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102921\
 Data File : VV023095.D
 Acq On : 29 Oct 2021 11:12
 Operator : SY/MD
 Sample : VV1029MBL05
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK270

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
 Title : VOC Analysis

37	6.307	1634	1638	1643	rVB4	590	618	0.06%	0.007%
38	6.500	1696	1698	1701	rVB3	605	255	0.02%	0.003%
39	6.571	1717	1720	1723	rBV2	223	180	0.02%	0.002%
40	6.590	1723	1726	1729	rBV2	417	212	0.02%	0.003%
41	6.622	1733	1736	1737	rBV2	320	187	0.02%	0.002%
42	6.744	1772	1774	1777	rBV	176	131	0.01%	0.002%
43	6.783	1782	1786	1791	rBV2	533	436	0.04%	0.005%
44	6.989	1838	1850	1870	rBV	131523	241321	22.00%	2.897%
45	7.133	1893	1895	1898	rBV2	365	156	0.01%	0.002%
46	7.256	1931	1933	1936	rVB2	306	161	0.01%	0.002%
47	7.317	1940	1952	1969	rBV	505464	864225	78.78%	10.375%
48	7.519	2011	2015	2018	rVB2	820	492	0.04%	0.006%
49	7.622	2036	2047	2071	rBV	96541	169930	15.49%	2.040%
50	7.902	2132	2134	2137	rBV	316	179	0.02%	0.002%
51	7.918	2137	2139	2141	rVV	388	190	0.02%	0.002%
52	7.982	2154	2159	2160	rBV2	438	326	0.03%	0.004%
53	8.088	2181	2192	2228	rBV	306783	527754	48.11%	6.336%
54	8.381	2280	2283	2287	rBV2	522	425	0.04%	0.005%
55	8.506	2316	2322	2324	rBV4	477	432	0.04%	0.005%
56	8.590	2345	2348	2351	rBV2	535	280	0.03%	0.003%
57	8.629	2358	2360	2364	rVB2	475	337	0.03%	0.004%
58	8.741	2393	2395	2396	rBV	351	160	0.01%	0.002%
59	8.751	2396	2398	2402	rVB2	549	216	0.02%	0.003%
60	8.773	2402	2405	2408	rBV2	359	250	0.02%	0.003%
61	8.789	2408	2410	2413	rBV3	497	257	0.02%	0.003%
62	8.802	2413	2414	2417	rBV2	256	145	0.01%	0.002%
63	8.854	2418	2430	2455	rBV	489526	789723	71.98%	9.481%
64	9.018	2478	2481	2484	rBV2	896	655	0.06%	0.008%
65	9.121	2511	2513	2516	rBV	395	196	0.02%	0.002%
66	9.207	2538	2540	2546	rBV2	292	299	0.03%	0.004%
67	9.471	2620	2622	2625	rVB2	396	198	0.02%	0.002%
68	9.545	2643	2645	2646	rBV	474	231	0.02%	0.003%
69	9.580	2653	2656	2660	rBV3	513	371	0.03%	0.004%
70	9.667	2680	2683	2684	rBV2	283	136	0.01%	0.002%
71	9.818	2727	2730	2732	rBV2	342	216	0.02%	0.003%
72	9.924	2761	2763	2766	rBV2	274	139	0.01%	0.002%
73	9.992	2782	2784	2785	rBV	276	130	0.01%	0.002%
74	10.014	2789	2791	2792	rBV	366	134	0.01%	0.002%
75	10.124	2818	2825	2833	rVB4	2666	3898	0.36%	0.047%
76	10.159	2833	2836	2838	rVB3	240	135	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102921\
 Data File : VV023095.D
 Acq On : 29 Oct 2021 11:12
 Operator : SY/MD
 Sample : VV1029MBL05
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK270

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M

Title : VOC Analysis

77	10.217	2842	2854	2875	rBV	356572	558219	50.88%	6.702%
78	10.458	2926	2929	2934	rVB3	479	418	0.04%	0.005%
79	10.484	2934	2937	2939	rBV2	379	310	0.03%	0.004%
80	10.545	2954	2956	2959	rBV2	382	283	0.03%	0.003%
81	10.657	2987	2991	2995	rBV5	587	391	0.04%	0.005%
82	10.789	3030	3032	3035	rBV2	295	177	0.02%	0.002%
83	10.828	3042	3044	3046	rVB	484	174	0.02%	0.002%
84	10.915	3065	3071	3086	rVB7	2303	3591	0.33%	0.043%
85	10.976	3086	3090	3091	rBV2	406	212	0.02%	0.003%
86	11.249	3164	3175	3196	rBV	487858	753575	68.69%	9.047%
87	11.545	3265	3267	3269	rBV	418	233	0.02%	0.003%
88	11.625	3280	3292	3311	rBV	520988	814467	74.24%	9.778%
89	11.847	3359	3361	3362	rBV	598	224	0.02%	0.003%
90	12.075	3428	3432	3434	rBV2	243	215	0.02%	0.003%
91	12.188	3465	3467	3470	rBV	212	146	0.01%	0.002%
92	12.596	3591	3594	3597	rBV2	604	404	0.04%	0.005%
93	12.792	3652	3655	3661	rVB2	369	263	0.02%	0.003%
94	12.969	3707	3710	3714	rBV2	311	271	0.02%	0.003%
95	13.040	3730	3732	3735	rBV3	293	145	0.01%	0.002%
96	13.114	3752	3755	3757	rBV2	374	196	0.02%	0.002%
97	13.175	3772	3774	3776	rBV	407	214	0.02%	0.003%
98	13.702	3936	3938	3942	rVB3	526	271	0.02%	0.003%
99	13.744	3947	3951	3952	rBV3	916	573	0.05%	0.007%
100	13.780	3959	3962	3967	rBV2	429	340	0.03%	0.004%




Sum of corrected areas: 8329570

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102921\
Data File : VV023095.D
Acq On : 29 Oct 2021 11:12
Operator : SY/MD
Sample : VV1029MBL05
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK270

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

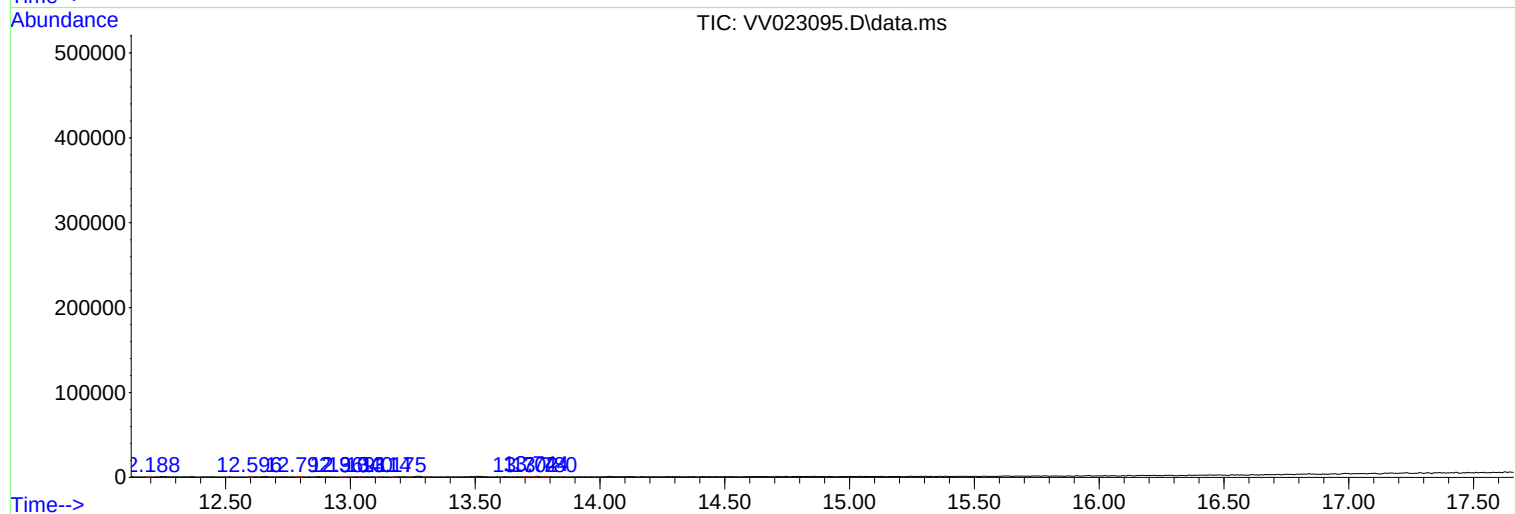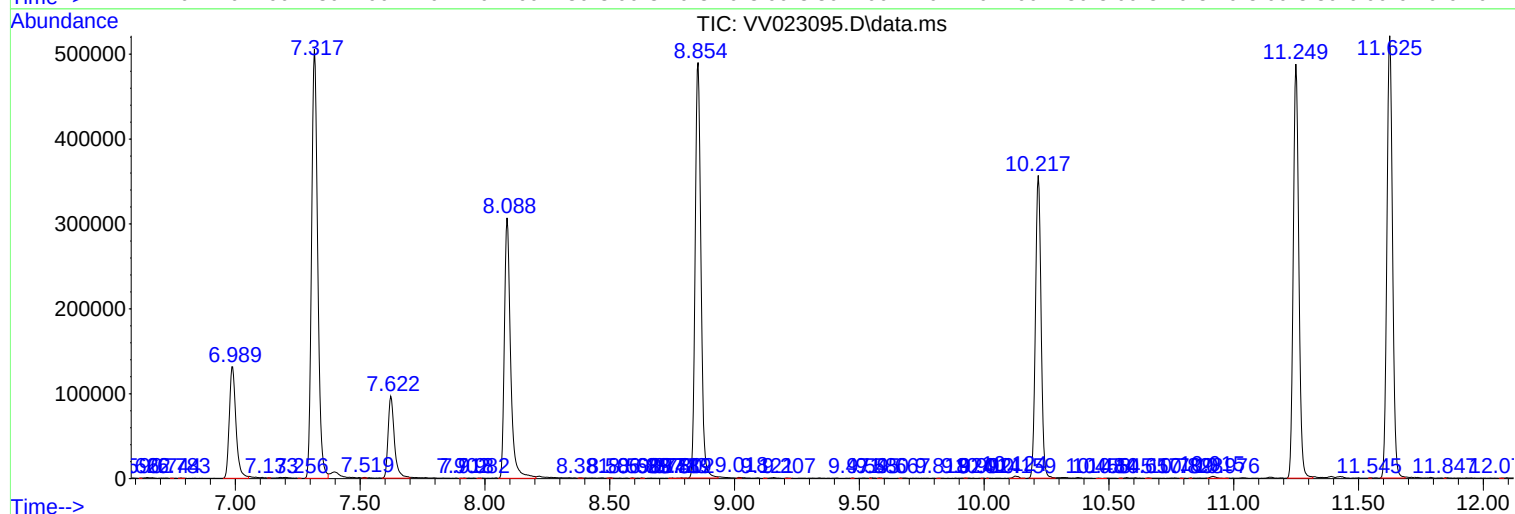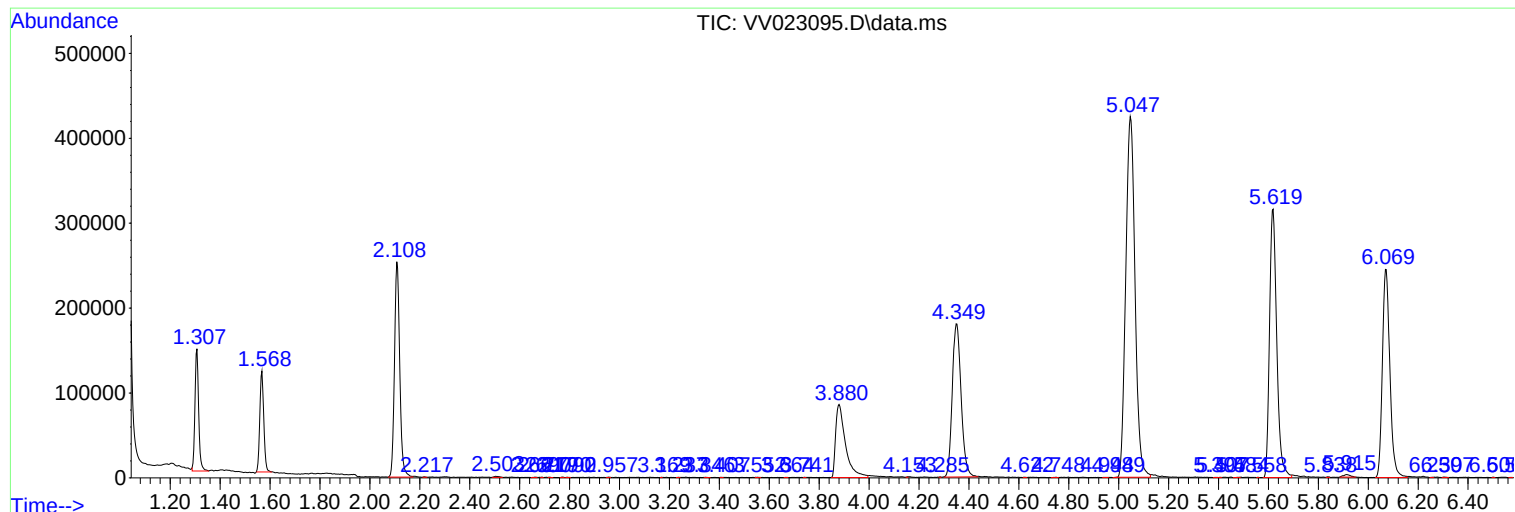

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102921\
Data File : VV023095.D
Acq On : 29 Oct 2021 11:12
Operator : SY/MD
Sample : VV1029MBL05
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK270

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102921\
Data File : VV023095.D
Acq On : 29 Oct 2021 11:12
Operator : SY/MD
Sample : VV1029MBL05
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK270

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
