

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102921\
 Data File : VV023097.D
 Acq On : 29 Oct 2021 11:58
 Operator : SY/MD
 Sample : VV1029WBL04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK272

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M

Title : VOC Analysis

Signal : TIC: VV023097.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	96	rVB	136669	141552	12.99%	1.717%
2	1.568	157	164	178	rVB	120076	135159	12.40%	1.639%
3	2.108	317	332	353	rBV	251171	366510	33.63%	4.446%
4	2.343	403	405	407	rVV	433	231	0.02%	0.003%
5	2.510	449	457	467	rVB5	1820	3068	0.28%	0.037%
6	2.831	553	557	560	rBV3	435	209	0.02%	0.003%
7	2.863	563	567	569	rBV	396	283	0.03%	0.003%
8	2.973	598	601	605	rBV3	396	333	0.03%	0.004%
9	3.037	618	621	627	rVB3	477	375	0.03%	0.005%
10	3.182	663	666	670	rVB3	358	268	0.02%	0.003%
11	3.211	673	675	681	rVB3	457	322	0.03%	0.004%
12	3.368	718	724	726	rBV3	313	292	0.03%	0.004%
13	3.439	742	746	751	rVB2	311	284	0.03%	0.003%
14	3.555	777	782	785	rBV3	315	308	0.03%	0.004%
15	3.648	809	811	815	rVB3	491	222	0.02%	0.003%
16	3.732	833	837	839	rBV2	272	190	0.02%	0.002%
17	3.806	856	860	862	rBV3	309	209	0.02%	0.003%
18	3.879	873	883	914	rBV	86555	231530	21.24%	2.808%
19	4.352	1013	1030	1052	rBV	187379	446974	41.01%	5.422%
20	4.587	1100	1103	1106	rBV3	643	583	0.05%	0.007%
21	4.622	1112	1114	1117	rBV	512	359	0.03%	0.004%
22	4.674	1127	1130	1134	rVB4	756	552	0.05%	0.007%
23	4.712	1136	1142	1145	rBV3	403	379	0.03%	0.005%
24	4.796	1165	1168	1171	rBV	336	203	0.02%	0.002%
25	4.834	1177	1180	1185	rBV3	266	194	0.02%	0.002%
26	4.896	1196	1199	1203	rBV3	574	386	0.04%	0.005%
27	4.921	1203	1207	1209	rBV3	370	278	0.03%	0.003%
28	4.957	1216	1218	1224	rVB3	266	210	0.02%	0.003%
29	5.047	1229	1246	1275	rBV3	423756	1089871	100.00%	13.220%
30	5.381	1347	1350	1353	rVB3	352	284	0.03%	0.003%
31	5.400	1353	1356	1357	rBV	318	199	0.02%	0.002%
32	5.513	1387	1391	1394	rBV3	352	315	0.03%	0.004%
33	5.555	1399	1404	1405	rBV	329	229	0.02%	0.003%
34	5.619	1411	1424	1450	rBV	309805	627062	57.54%	7.606%
35	5.918	1506	1517	1528	rBV5	3221	7045	0.65%	0.085%
36	6.069	1548	1564	1591	rBV	244225	502049	46.06%	6.090%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102921\
 Data File : VV023097.D
 Acq On : 29 Oct 2021 11:58
 Operator : SY/MD
 Sample : VV1029WBL04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK272

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
 Title : VOC Analysis

37	6.407	1665	1669	1673	rVB4	437	383	0.04%	0.005%
38	6.436	1673	1678	1679	rBV	337	229	0.02%	0.003%
39	6.535	1705	1709	1711	rBV3	499	331	0.03%	0.004%
40	6.638	1733	1741	1743	rBV5	526	725	0.07%	0.009%
41	6.828	1795	1800	1803	rVB3	420	327	0.03%	0.004%
42	6.854	1803	1808	1810	rBV	317	206	0.02%	0.002%
43	6.985	1838	1849	1869	rBV	130151	236557	21.71%	2.869%
44	7.317	1940	1952	1971	rBV	501168	860971	79.00%	10.443%
45	7.567	2028	2030	2036	rVB4	493	425	0.04%	0.005%
46	7.622	2036	2047	2076	rBV	94522	168870	15.49%	2.048%
47	7.895	2128	2132	2136	rVB3	595	349	0.03%	0.004%
48	7.918	2136	2139	2141	rBV2	356	206	0.02%	0.002%
49	7.934	2141	2144	2146	rBV2	398	201	0.02%	0.002%
50	7.966	2152	2154	2158	rVB2	359	204	0.02%	0.002%
51	8.088	2181	2192	2227	rBV	298623	519375	47.65%	6.300%
52	8.352	2271	2274	2278	rBV2	539	353	0.03%	0.004%
53	8.436	2298	2300	2302	rBV	304	213	0.02%	0.003%
54	8.545	2330	2334	2337	rBV2	494	356	0.03%	0.004%
55	8.580	2340	2345	2348	rBV3	576	552	0.05%	0.007%
56	8.854	2418	2430	2449	rBV	475056	771462	70.78%	9.358%
57	9.104	2505	2508	2509	rBV2	470	204	0.02%	0.002%
58	9.278	2560	2562	2567	rVB2	387	217	0.02%	0.003%
59	9.333	2576	2579	2581	rBV	450	236	0.02%	0.003%
60	9.448	2612	2615	2617	rBV	358	208	0.02%	0.003%
61	9.464	2617	2620	2626	rVB3	325	250	0.02%	0.003%
62	9.628	2668	2671	2677	rVB2	303	260	0.02%	0.003%
63	9.664	2680	2682	2685	rBV2	446	189	0.02%	0.002%
64	9.722	2696	2700	2703	rBV2	318	242	0.02%	0.003%
65	9.747	2703	2708	2711	rBV2	435	297	0.03%	0.004%
66	9.902	2753	2756	2759	rBV2	271	194	0.02%	0.002%
67	9.947	2766	2770	2771	rBV2	436	301	0.03%	0.004%
68	9.998	2781	2786	2788	rBV2	377	254	0.02%	0.003%
69	10.127	2814	2826	2834	rBV5	2512	4014	0.37%	0.049%
70	10.217	2842	2854	2871	rBV	356551	550948	50.55%	6.683%
71	10.317	2883	2885	2889	rBV3	603	373	0.03%	0.005%
72	10.439	2922	2923	2926	rBV	387	239	0.02%	0.003%
73	10.574	2957	2965	2967	rBV4	807	937	0.09%	0.011%
74	10.603	2972	2974	2979	rVB3	528	355	0.03%	0.004%
75	10.641	2982	2986	2988	rBV3	302	209	0.02%	0.003%
76	10.661	2988	2992	2995	rBV2	330	199	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102921\
 Data File : VV023097.D
 Acq On : 29 Oct 2021 11:58
 Operator : SY/MD
 Sample : VV1029WBL04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK272

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
 Title : VOC Analysis

77	10.715	3006	3009	3012	rBV2	253	192	0.02%	0.002%
78	10.789	3030	3032	3036	rBV2	322	211	0.02%	0.003%
79	10.918	3066	3072	3081	rVB6	2245	2807	0.26%	0.034%
80	11.024	3102	3105	3108	rBV	304	232	0.02%	0.003%
81	11.143	3138	3142	3144	rBV2	1016	908	0.08%	0.011%
82	11.249	3164	3175	3194	rBV	489239	742171	68.10%	9.002%
83	11.577	3274	3277	3280	rBV2	699	529	0.05%	0.006%
84	11.625	3280	3292	3313	rVV	523846	811315	74.44%	9.841%
85	12.027	3412	3417	3420	rBV2	346	370	0.03%	0.004%
86	12.220	3472	3477	3480	rBV3	456	427	0.04%	0.005%
87	12.387	3523	3529	3531	rBV3	351	333	0.03%	0.004%
88	12.879	3679	3682	3685	rBV2	364	220	0.02%	0.003%
89	13.030	3727	3729	3735	rVB3	391	304	0.03%	0.004%
90	13.123	3756	3758	3763	rVV4	502	381	0.03%	0.005%
91	13.259	3797	3800	3801	rBV2	351	199	0.02%	0.002%
92	13.371	3832	3835	3839	rBV2	386	270	0.02%	0.003%
93	13.461	3860	3863	3865	rBV2	346	240	0.02%	0.003%
94	13.844	3979	3982	3984	rBV	342	270	0.02%	0.003%
95	13.869	3988	3990	3994	rVB2	462	273	0.03%	0.003%
96	14.043	4040	4044	4049	rBV2	611	668	0.06%	0.008%
97	14.384	4148	4150	4152	rBV	415	212	0.02%	0.003%
98	14.606	4216	4219	4221	rBV3	486	264	0.02%	0.003%
99	14.628	4223	4226	4228	rBV2	380	222	0.02%	0.003%
100	15.410	4467	4469	4471	rBV2	518	242	0.02%	0.003%




Sum of corrected areas: 8244198

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102921\
Data File : VV023097.D
Acq On : 29 Oct 2021 11:58
Operator : SY/MD
Sample : VV1029WBL04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK272

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

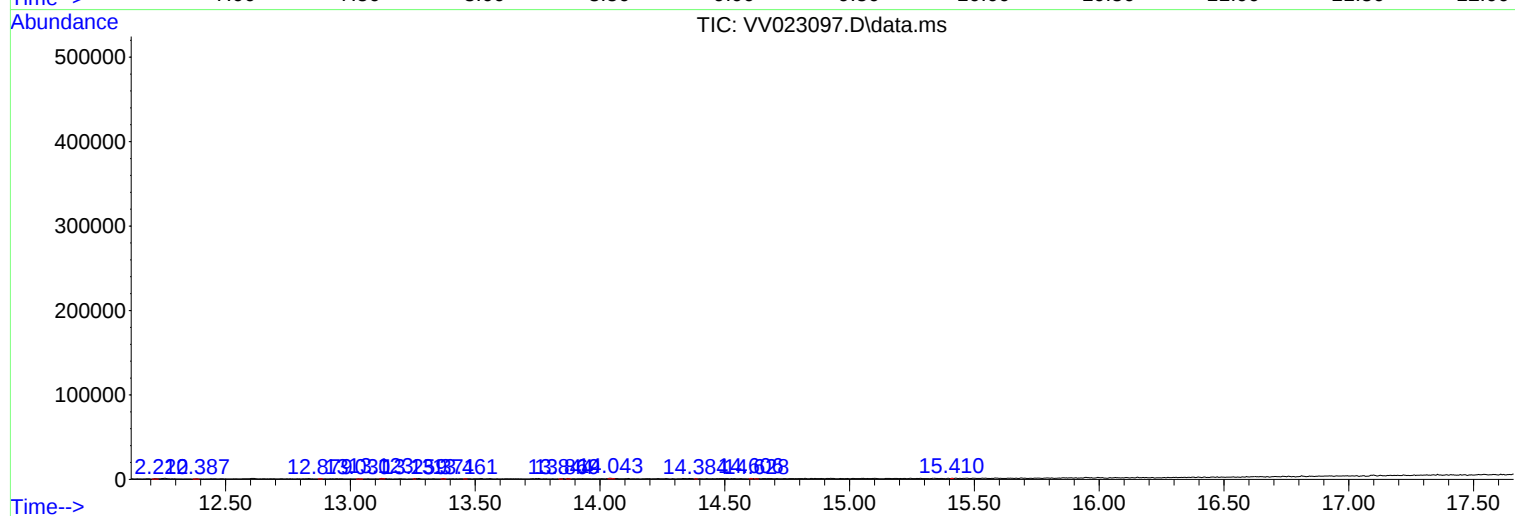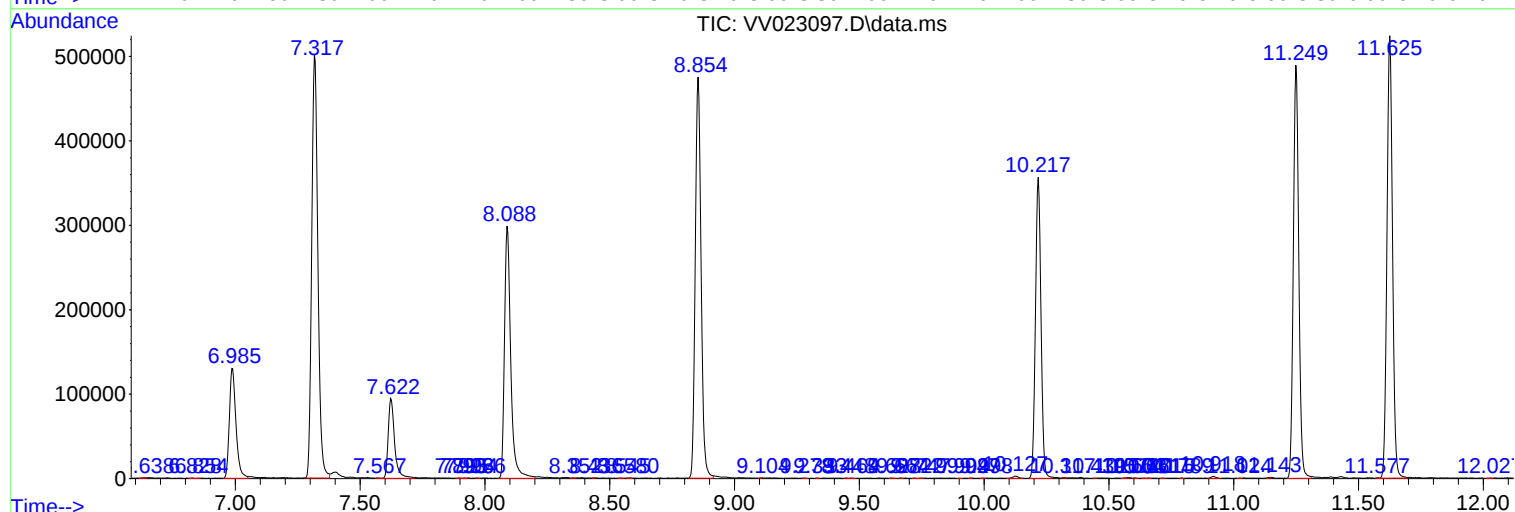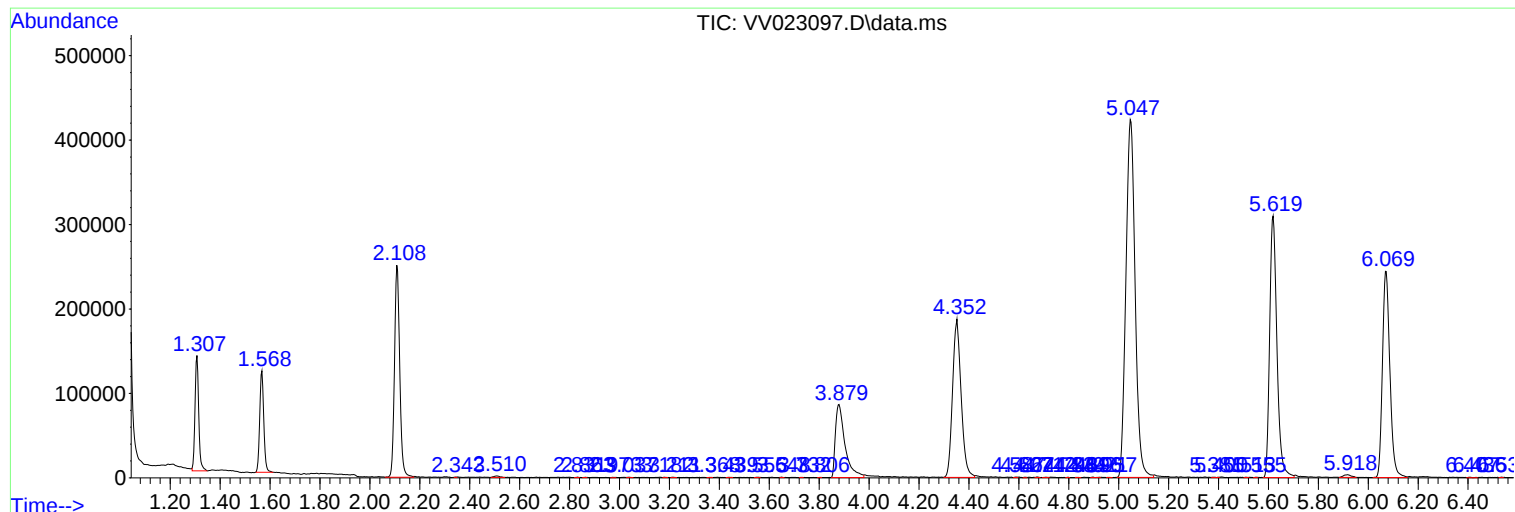

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102921\
Data File : VV023097.D
Acq On : 29 Oct 2021 11:58
Operator : SY/MD
Sample : VV1029WBL04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK272

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102921\
Data File : VV023097.D
Acq On : 29 Oct 2021 11:58
Operator : SY/MD
Sample : VV1029WBL04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK272

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
