
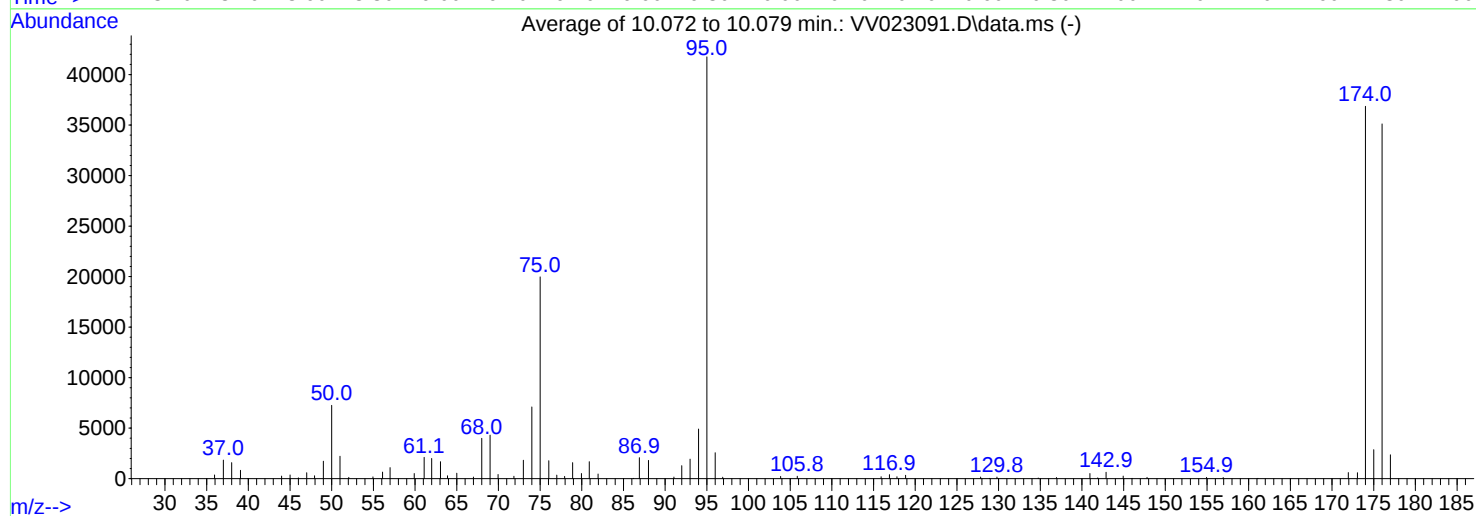


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102921\
 Data File : VV023091.D
 Acq On : 29 Oct 2021 09:11
 Operator : SY/MD
 Sample : BFB244
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB244

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
 Title : VOC Analysis
 Last Update : Sat Oct 30 00:25:16 2021

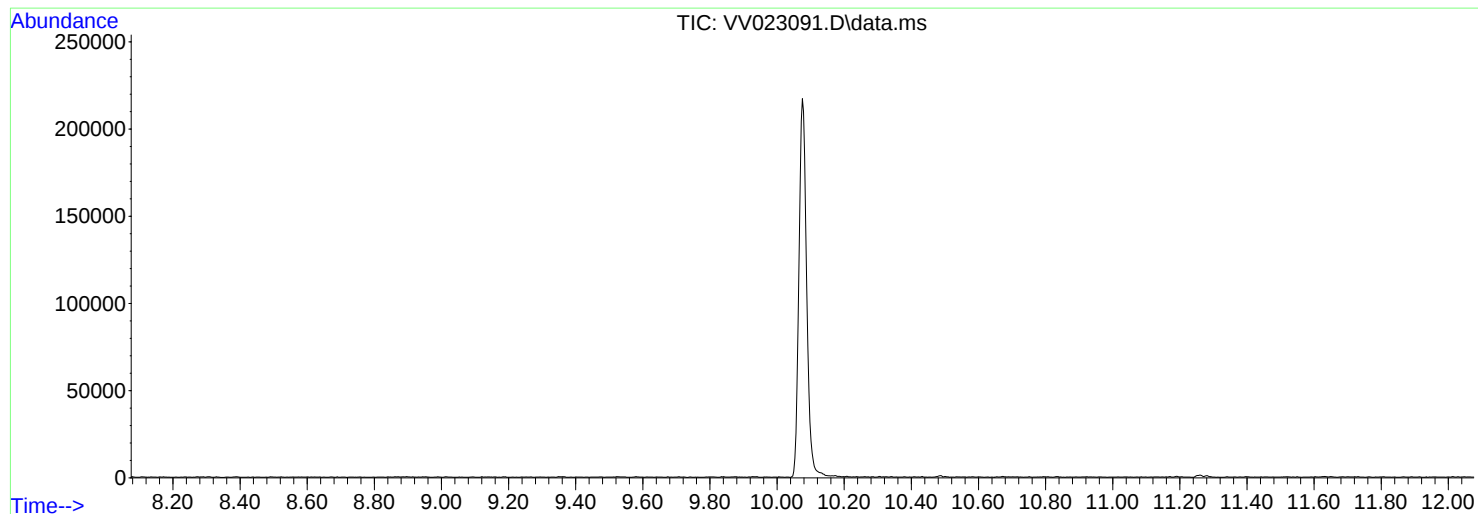

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	7261	PASS
75	95	30	80	47.8	19976	PASS
95	95	100	100	100.0	41755	PASS
96	95	5	9	6.1	2564	PASS
173	174	0.00	2	1.6	584	PASS
174	95	50	120	88.3	36859	PASS
175	174	5	9	7.8	2872	PASS
176	174	95	105	95.3	35117	PASS
177	176	5	10	6.7	2369	PASS

m/z	Abundance
35.90	323.0
37.00	1749.0
38.00	1586.0
39.00	802.0
39.90	218.0
44.00	394.0
45.00	387.0
47.00	580.0
47.90	299.0
49.00	1779.0
50.00	6949.0
51.00	2165.0
52.00	125.0
54.90	137.0
56.10	602.0
57.00	1054.0
59.90	473.0
61.10	2027.0
62.00	2020.0
63.00	1750.0
63.90	300.0
65.00	512.0
67.00	157.0
68.00	4027.0
69.00	4368.0
70.00	405.0
71.80	233.0
73.00	1840.0
74.00	6980.0
75.00	19472.0
76.00	1814.0
77.00	382.0
77.90	193.0
78.90	1489.0
80.00	469.0
80.90	1720.0
82.00	497.0
86.90	1987.0
88.00	1840.0
91.00	154.0
92.00	1257.0
93.00	1987.0
94.00	4896.0
95.00	41328.0
96.00	2511.0
96.90	112.0
103.80	232.0
105.80	265.0
115.90	227.0
116.90	355.0
117.80	164.0
118.80	345.0
127.90	160.0
128.90	123.0
129.80	178.0
134.80	109.0
137.00	101.0
141.00	500.0
141.90	112.0
142.90	617.0
144.90	278.0
147.80	145.0
154.90	135.0
157.00	102.0
171.90	674.0
173.10	616.0
174.00	37576.0
175.00	2731.0
176.00	35584.0
177.00	2315.0

Instrument :
MSVOA_V
ClientSampleId :
BFB244

Scan 2798 (10.037 min): VV023091.D\data.ms
BFB244

m/z	Abundance
40.10	189.0
44.00	180.0

Instrument :
MSVOA_V
ClientSampleId :
BFB244

m/z	Abundance
36.00	393.0
37.00	1888.0
38.00	1535.0
39.10	825.0
39.90	197.0
44.00	464.0
45.00	344.0
46.00	118.0
47.00	576.0
48.00	284.0
49.00	1587.0
50.00	7299.0
51.00	2218.0
52.10	124.0
55.00	204.0
56.10	696.0
57.00	1127.0
59.90	508.0
61.10	2085.0
62.00	1897.0
63.10	1548.0
63.90	270.0
65.00	531.0
67.00	163.0
68.00	3865.0
69.00	4142.0
69.90	393.0
72.00	228.0
73.00	1766.0
74.00	6932.0
75.00	19968.0
76.10	1665.0
77.00	292.0
78.00	238.0
78.90	1613.0
79.90	540.0
80.90	1567.0
81.90	413.0
86.20	109.0
86.90	2075.0
88.00	1713.0
91.00	154.0
92.00	1301.0
93.00	1794.0
94.00	4814.0
95.00	40768.0
96.00	2559.0
96.90	172.0
103.90	212.0
105.80	205.0
115.90	156.0
116.90	425.0
117.80	213.0
118.90	301.0
127.80	153.0
129.80	156.0
136.90	125.0
140.90	479.0
142.90	637.0
145.00	248.0
146.00	124.0
147.80	109.0
155.00	112.0
156.90	110.0
161.10	114.0
172.00	516.0
173.00	529.0
174.00	34984.0
175.00	2910.0
176.00	33384.0
177.00	2348.0

Instrument :
MSVOA_V
ClientSampleId :
BFB244

m/z	Abundance
35.90	387.0
37.00	1867.0
38.00	1632.0
39.10	856.0
39.90	206.0
44.00	432.0
45.00	367.0
46.00	107.0
47.00	628.0
48.00	296.0
49.00	1815.0
50.00	7536.0
51.00	2288.0
52.10	110.0
55.00	196.0
56.10	660.0
57.00	1111.0
59.90	522.0
61.10	2195.0
62.00	2060.0
63.00	1720.0
63.90	306.0
65.00	598.0
67.00	171.0
68.00	4082.0
69.00	4412.0
70.00	423.0
71.80	249.0
73.00	1842.0
74.00	7388.0
75.00	20488.0
76.00	1837.0
77.00	367.0
78.00	243.0
78.90	1642.0
79.90	524.0
80.90	1758.0
81.90	465.0
86.90	2184.0
88.00	1859.0
91.10	155.0
92.00	1316.0
93.00	2006.0
94.00	5001.0
95.00	43168.0
96.00	2622.0
96.90	160.0
103.90	218.0
105.90	252.0
115.90	206.0
116.90	411.0
117.80	209.0
118.90	341.0
127.90	165.0
129.80	158.0
134.70	104.0
137.00	121.0
141.00	526.0
141.90	106.0
142.90	645.0
145.00	251.0
147.80	129.0
155.00	139.0
157.00	106.0
172.00	628.0
173.00	607.0
174.00	38016.0
175.00	2974.0
176.00	36384.0
177.00	2445.0

Instrument :
MSVOA_V
ClientSampleId :
BFB244