
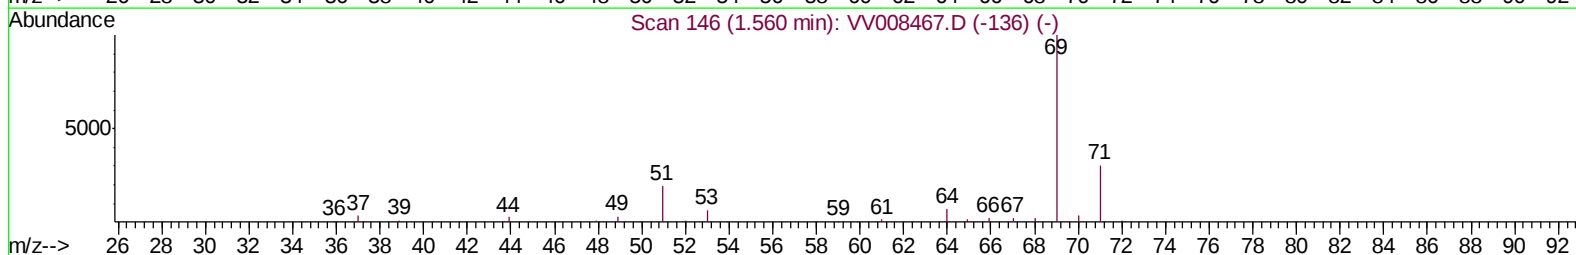
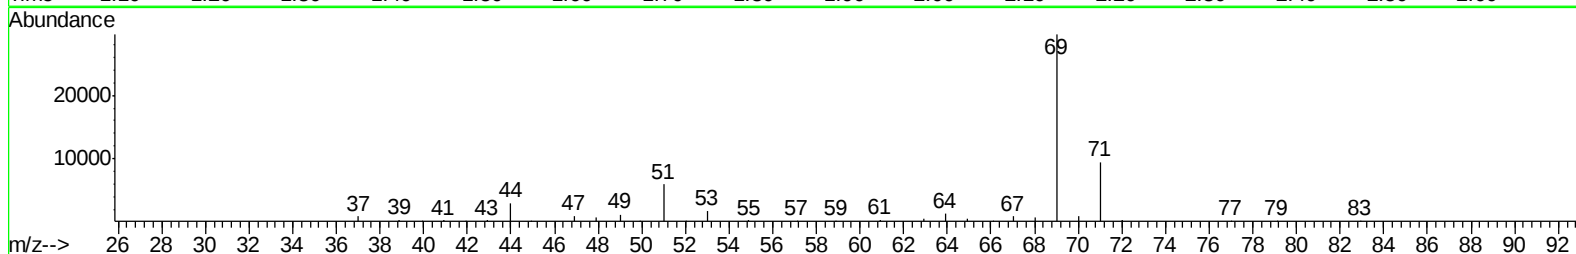


Data File : VV008477.D
Acq On : 30 Oct 2018 18:57
Operator : SY/MD
Sample : J5716-16
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Oct 31 08:23:02 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 31 07:14:32 2018
Response via : Initial Calibration

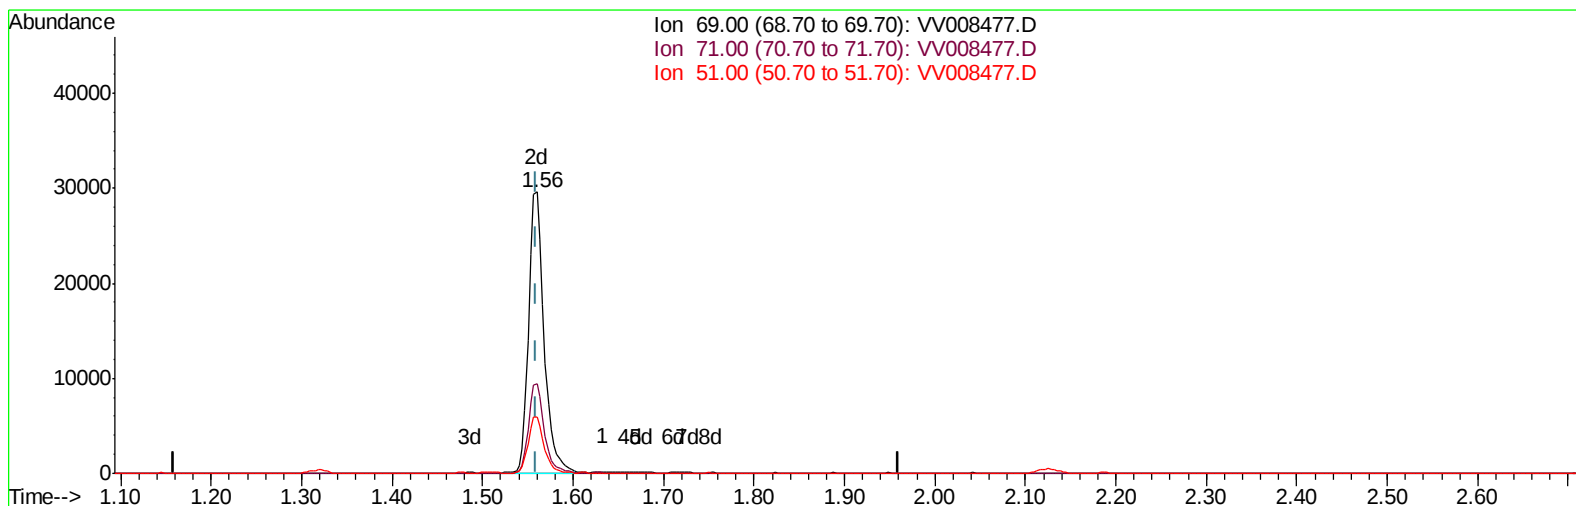

TIC: VV008477.D

(7) Chloroethane-d5 (S)

1.560min (-0.000) 47.78ug/L m

response 35213

Ion	Exp%	Act%
69.00	100	100
71.00	32.60	0.18#
51.00	29.80	0.20#
0.00	0.00	0.00