


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV103018\
Data File : VV008466.D
Acq On : 30 Oct 2018 14:07
Operator : SY/MD
Sample : BFB53
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB53

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
Title : VOC Analysis
Last Update : Wed Oct 31 07:14:32 2018

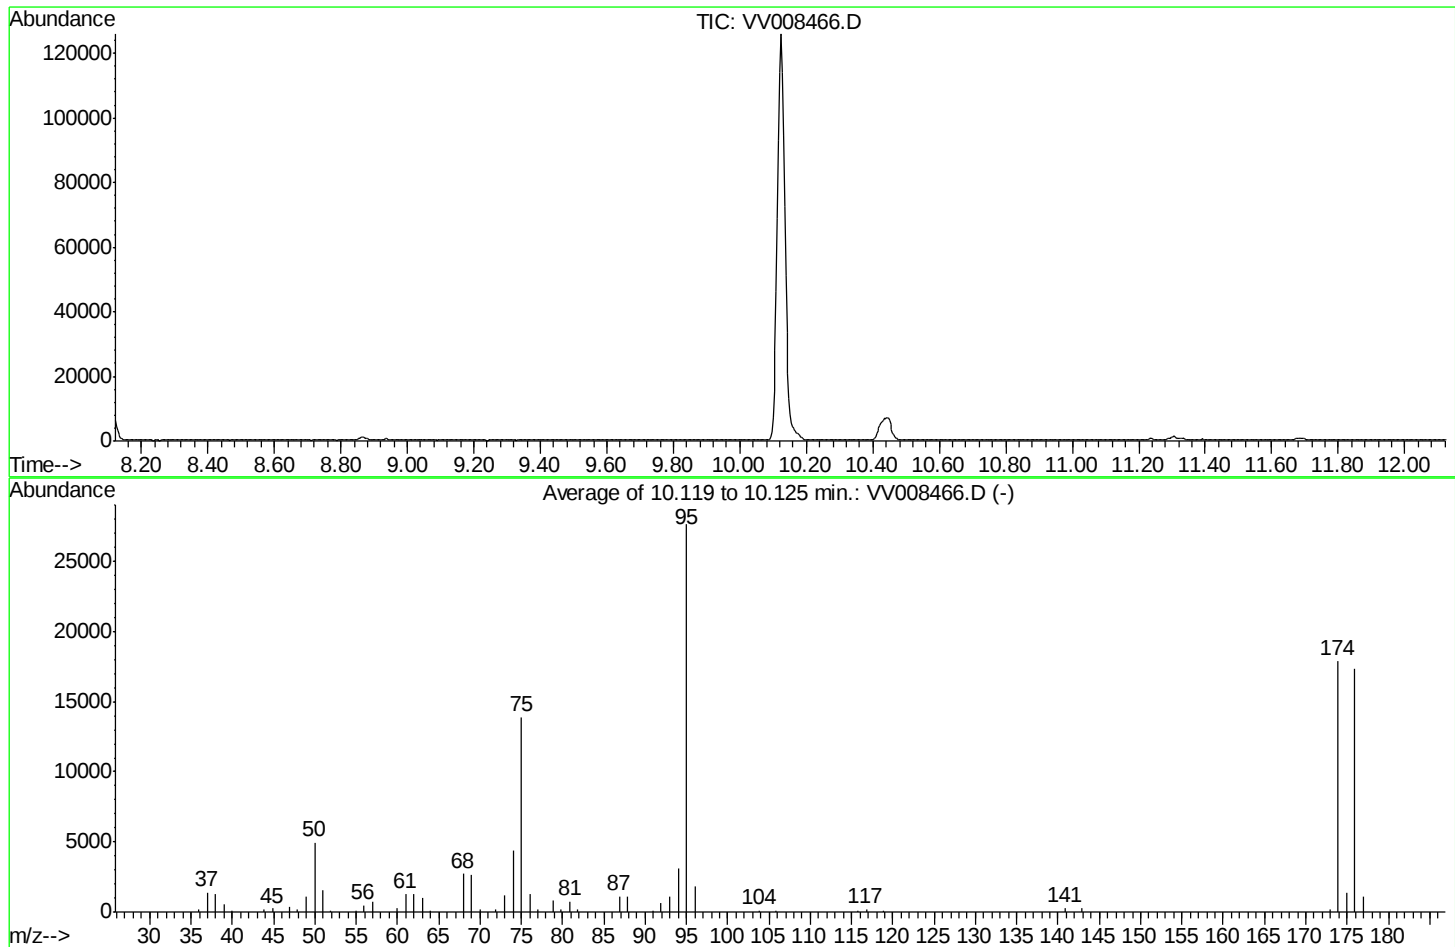

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	4972	PASS
75	95	30	80	50.2	13890	PASS
95	95	100	100	100.0	27642	PASS
96	95	5	9	6.7	1857	PASS
173	174	0.00	2	0.9	154	PASS
174	95	50	120	64.7	17898	PASS
175	174	5	9	7.6	1367	PASS
176	174	95	101	96.7	17304	PASS
177	176	5	9	6.2	1079	PASS

m/z	Abundance
43.90	214.0

Instrument :
MSVOA_V
ClientSampleId :
BFB53

m/z	Abundance
35.90	183.0
37.00	1370.0
38.00	1198.0
38.90	501.0
39.90	136.0
43.90	403.0
44.90	231.0
46.90	305.0
47.90	184.0
49.00	1085.0
50.00	4671.0
51.00	1504.0
54.90	104.0
55.90	431.0
57.00	746.0
59.90	242.0
61.00	1202.0
62.00	1242.0
63.00	961.0
63.90	103.0
68.00	2559.0
69.00	2522.0
70.00	160.0
71.80	136.0
73.00	1175.0
74.00	4188.0
75.00	12943.0
76.00	1269.0
77.10	201.0
78.90	750.0
79.80	211.0
80.90	698.0
81.80	158.0
86.90	1064.0
87.90	965.0
91.00	124.0
92.00	620.0
93.00	1082.0
94.00	2840.0
95.00	26176.0
96.00	1811.0
103.80	110.0
115.80	103.0
116.80	188.0
118.90	107.0
140.90	287.0
142.90	242.0
173.90	16536.0
175.00	1221.0
175.90	15872.0
176.90	998.0

Instrument :
MSVOA_V
ClientSampleId :
BFB53

m/z	Abundance
35.90	202.0
37.00	1430.0
38.00	1278.0
39.00	527.0
39.90	124.0
44.00	372.0
44.90	262.0
46.90	337.0
47.90	216.0
49.00	1162.0
50.00	5115.0
51.00	1634.0
51.80	106.0
55.00	113.0
55.90	493.0
57.00	719.0
59.90	251.0
61.00	1314.0
62.00	1330.0
63.00	1024.0
63.90	103.0
68.00	2818.0
69.00	2734.0
70.00	213.0
71.90	159.0
73.00	1265.0
74.00	4539.0
75.00	14347.0
76.00	1316.0
77.10	203.0
78.90	838.0
79.90	206.0
80.90	772.0
81.80	162.0
86.90	1178.0
87.90	1102.0
91.00	115.0
92.00	642.0
93.00	1185.0
94.00	3195.0
95.00	28544.0
96.00	1935.0
103.80	122.0
105.90	117.0
115.80	128.0
116.80	224.0
118.80	117.0
140.90	305.0
142.90	279.0
173.00	219.0
174.00	18472.0
175.00	1404.0
175.90	17928.0
176.90	1099.0

Instrument :
MSVOA_V
ClientSampleId :
BFB53

m/z	Abundance
35.90	193.0
37.00	1344.0
38.00	1236.0
39.00	499.0
39.90	109.0
44.00	384.0
44.90	254.0
46.90	330.0
47.90	203.0
49.00	1077.0
50.00	5130.0
51.00	1614.0
51.90	100.0
55.00	114.0
55.90	469.0
57.00	652.0
59.90	237.0
61.00	1337.0
62.00	1256.0
63.00	1006.0
68.00	2788.0
69.00	2730.0
70.00	244.0
71.90	167.0
73.00	1267.0
74.00	4509.0
75.00	14381.0
76.00	1240.0
77.00	170.0
78.90	825.0
79.90	199.0
80.90	742.0
81.90	163.0
86.90	1142.0
87.90	1096.0
90.80	109.0
91.90	662.0
93.00	1142.0
94.00	3263.0
95.00	28208.0
96.00	1827.0
103.90	131.0
105.90	136.0
115.80	138.0
116.80	192.0
118.90	123.0
140.90	297.0
142.90	297.0
172.90	244.0
174.00	18688.0
175.00	1478.0
175.90	18112.0
176.90	1140.0

Instrument :
MSVOA_V
ClientSampleId :
BFB53