
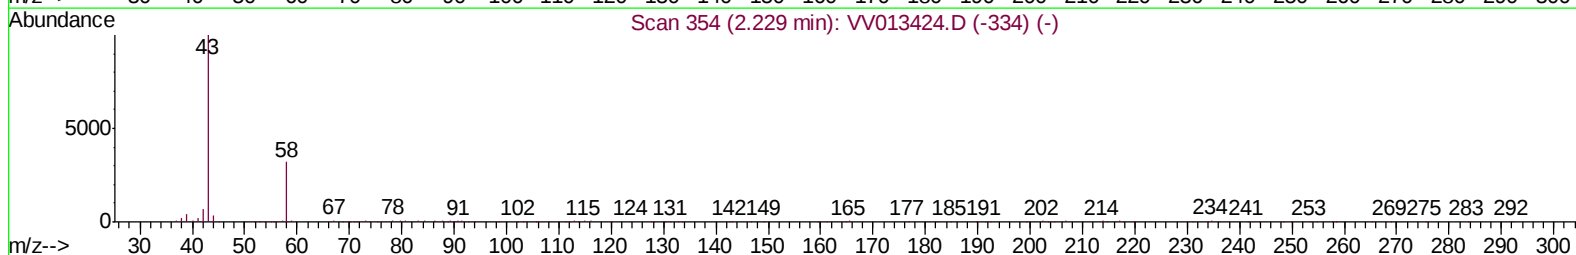
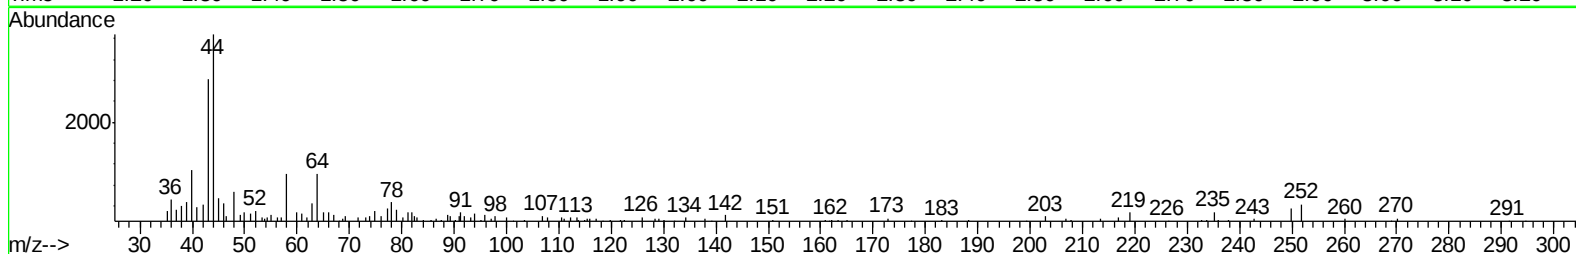


Data File : VV013432.D
Acq On : 30 Oct 2019 14:38
Operator : SY/MD
Sample : K5597-06
Misc : 25.0ML/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Oct 31 02:46:08 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Oct 31 02:41:56 2019
Response via : Initial Calibration

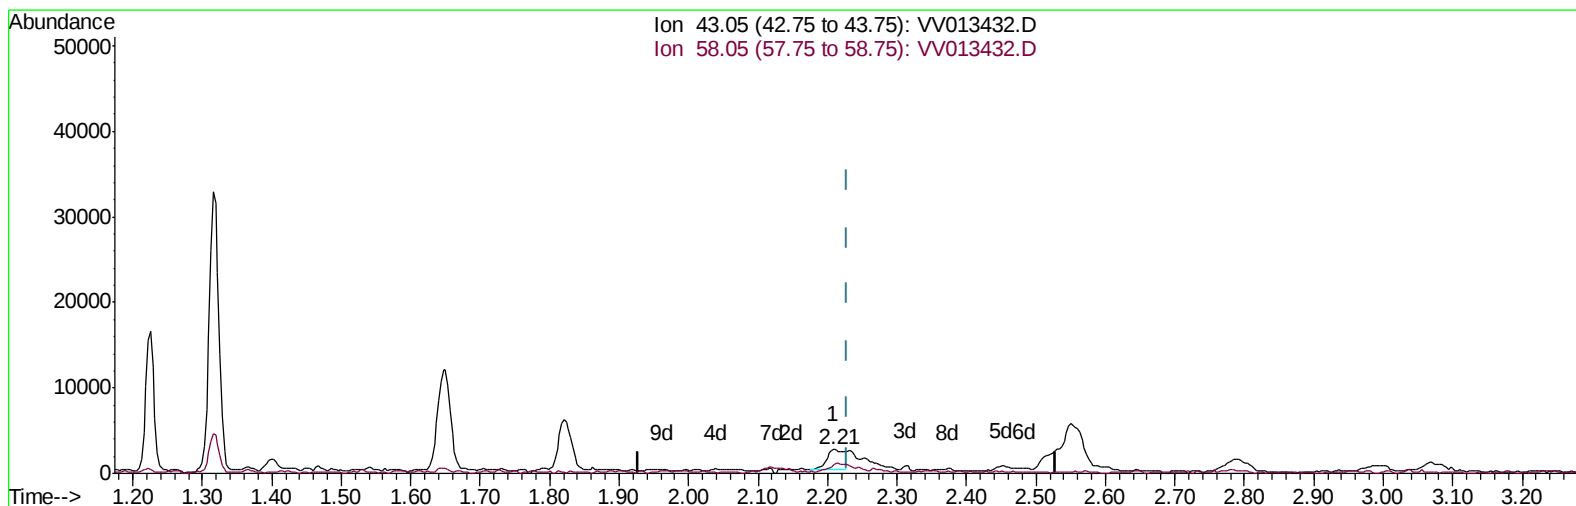

TIC: VV013432.D

(13) Acetone (T)

2.209min (-0.019) 1.12ug/L

response 4159

Ion	Exp%	Act%
43.05	100	100
58.05	29.50	29.24
0.00	0.00	0.00
0.00	0.00	0.00