

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV103019\
 Data File : VV013425.D
 Acq On : 30 Oct 2019 11:30
 Operator : SY/MD
 Sample : VV1030WBL01
 Misc : 25.0ML/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK44

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102919WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.116	5	8	17	rVB	30272	28760	1.65%	0.217%
2	1.225	36	42	48	rVB2	25360	25983	1.49%	0.196%
3	1.315	62	70	84	rBV	219571	236709	13.60%	1.785%
4	1.582	146	153	166	rBV	195127	229583	13.19%	1.731%
5	2.129	313	323	334	rVB	358904	501759	28.82%	3.783%
6	2.534	443	449	461	rVB2	14985	24436	1.40%	0.184%
7	3.965	878	894	938	rBV2	140884	694420	39.89%	5.235%
8	4.399	1012	1029	1052	rBV	300705	756161	43.43%	5.701%
9	5.093	1230	1245	1275	rBV3	723616	1741029	100.00%	13.126%
10	5.663	1406	1422	1442	rBV	410450	825273	47.40%	6.222%
11	5.949	1498	1511	1525	rVB5	18198	40740	2.34%	0.307%
12	6.116	1549	1563	1582	rBV	405597	818300	47.00%	6.169%
13	7.029	1837	1847	1863	rBV	196370	341837	19.63%	2.577%
14	7.357	1937	1949	1967	rBV	797746	1373098	78.87%	10.352%
15	7.663	2034	2044	2058	rBV	115906	201133	11.55%	1.516%
16	8.135	2179	2191	2223	rBV3	674524	1524860	87.58%	11.496%
17	8.894	2414	2427	2447	rBV	695364	1136957	65.30%	8.571%
18	10.257	2839	2851	2868	rBV	277766	438586	25.19%	3.306%
19	11.289	3161	3172	3191	rBV	729086	1145010	65.77%	8.632%
20	11.669	3276	3290	3305	rBV	735734	1179826	67.77%	8.895%


Sum of corrected areas: 13264460

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV103019\
Data File : VV013425.D
Acq On : 30 Oct 2019 11:30
Operator : SY/MD
Sample : VV1030WBL01
Misc : 25.0ML/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK44

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102919WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

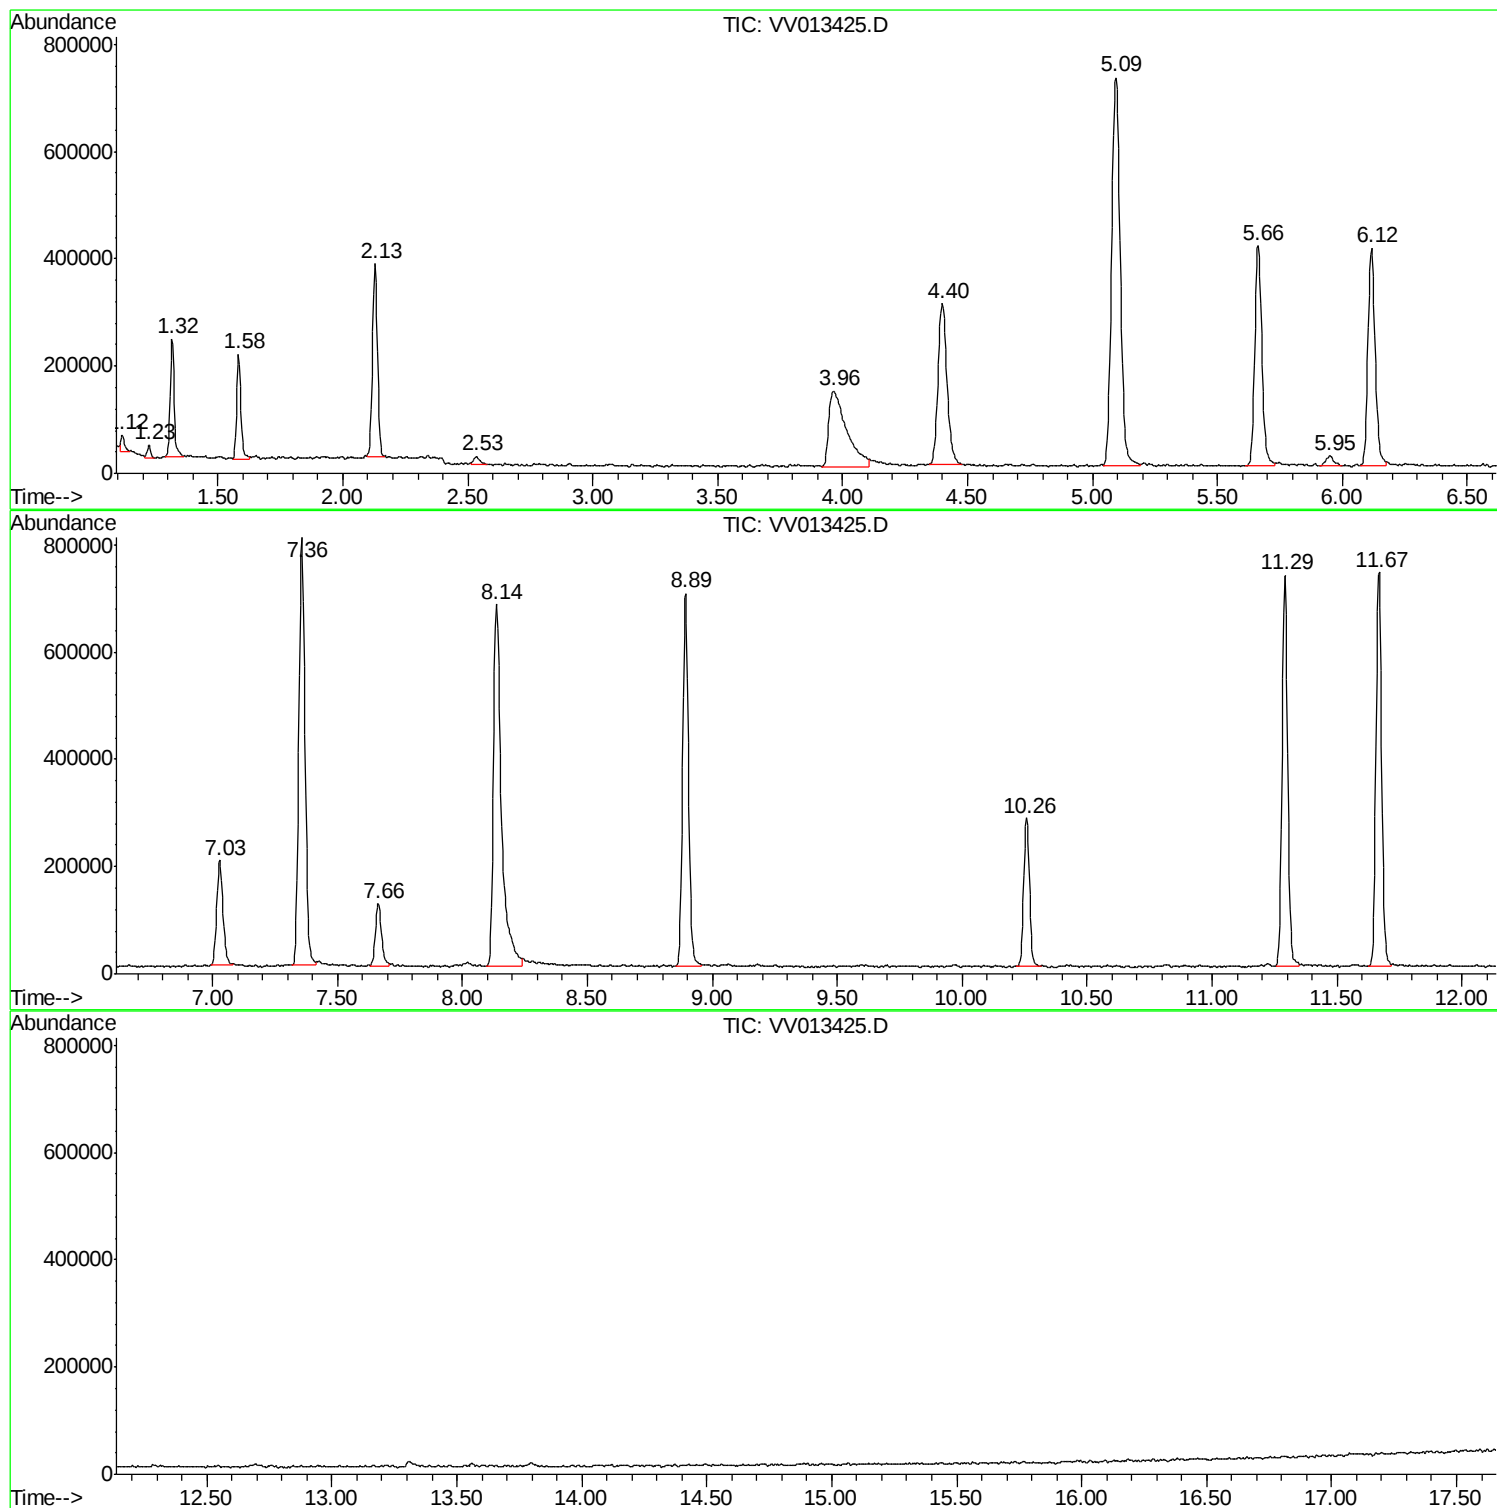

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV103019\
Data File : VV013425.D
Acq On : 30 Oct 2019 11:30
Operator : SY/MD
Sample : VV1030WBL01
Misc : 25.0ML/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK44










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102919WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.03	2.07 ug/L	341837	1,4-Difluorobenzene	5.66

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	32
2		Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	25
3		1,3-Cyclohexadiene	80	C6H8	000592-57-4	23
4		2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	23
5		2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	17

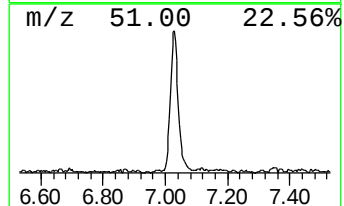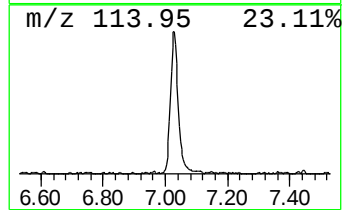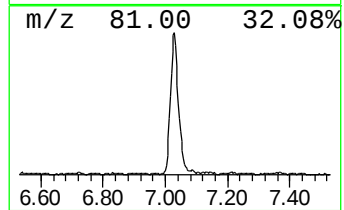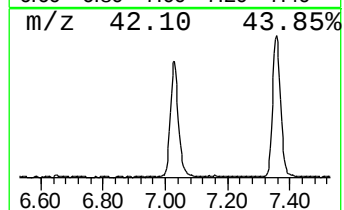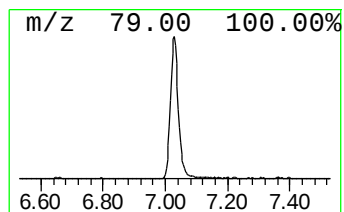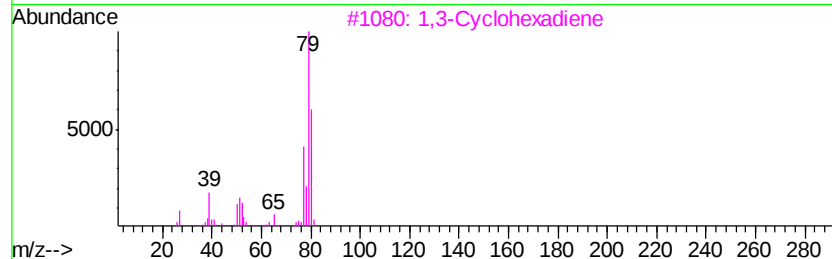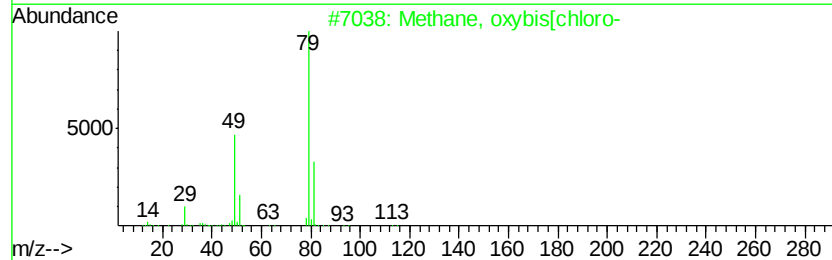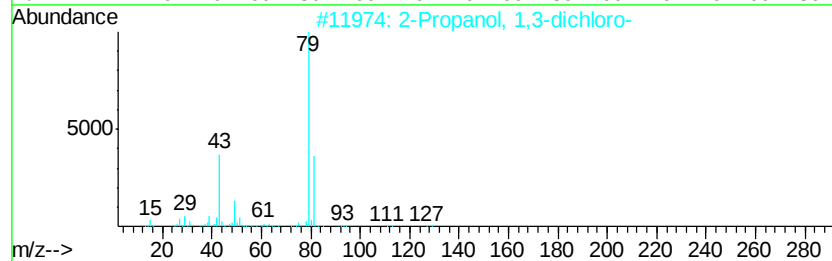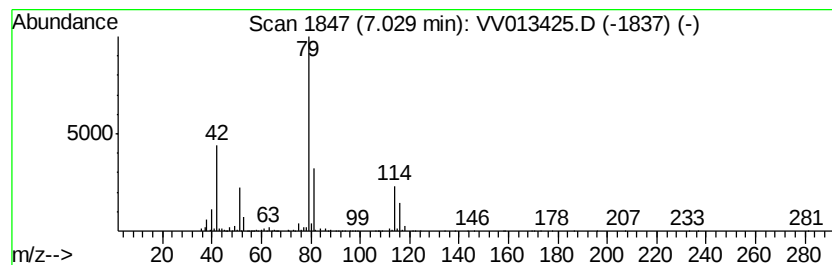

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV103019\
Data File : VV013425.D
Acq On : 30 Oct 2019 11:30
Operator : SY/MD
Sample : VV1030WBL01
Misc : 25.0ML/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK44

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102919WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	7.03	2.1	ug/L	341837	1	5.66	825273	5.0