

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV103020\
 Data File : VV019193.D
 Acq On : 30 Oct 2020 18:38
 Operator : SY/MD
 Sample : VIBLK64
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK64

Quant Time: Oct 31 04:28:36 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 31 02:55:48 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	221427	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	216483	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	106895	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	71003	40.35	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	80.70%
7) Chloroethane-d5	1.58	69	57588	42.13	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	84.26%
11) 1,1-Dichloroethene-d2	2.12	63	109075	32.58	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.16%
21) 2-Butanone-d5	3.91	46	96089	89.16	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.16%
24) Chloroform-d	4.38	84	146113	44.64	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.28%
26) 1,2-Dichloroethane-d4	5.05	65	107287	47.04	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.08%
32) Benzene-d6	5.07	84	280476	45.67	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.34%
36) 1,2-Dichloropropane-d6	6.09	67	86805	47.41	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.82%
41) Toluene-d8	7.34	98	258173	43.76	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.52%
43) trans-1,3-Dichloropropene-	7.64	79	46027	43.44	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.88%
47) 2-Hexanone-d5	8.11	63	65943	83.16	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	83.16%
57) 1,1,2,2-Tetrachloroethane-	10.23	84	107824	43.67	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	87.34%
64) 1,2-Dichlorobenzene-d4	11.65	152	110326	49.12	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.24%


Target Compounds					Ovalue
46) Tetrachloroethene	8.00	164	2401	1.644 ug/L	91




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV103020\
Data File : VV019193.D
Acq On : 30 Oct 2020 18:38
Operator : SY/MD
Sample : VIBLK64
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK64

Quant Time: Oct 31 04:28:36 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 31 02:55:48 2020
Response via : Initial Calibration

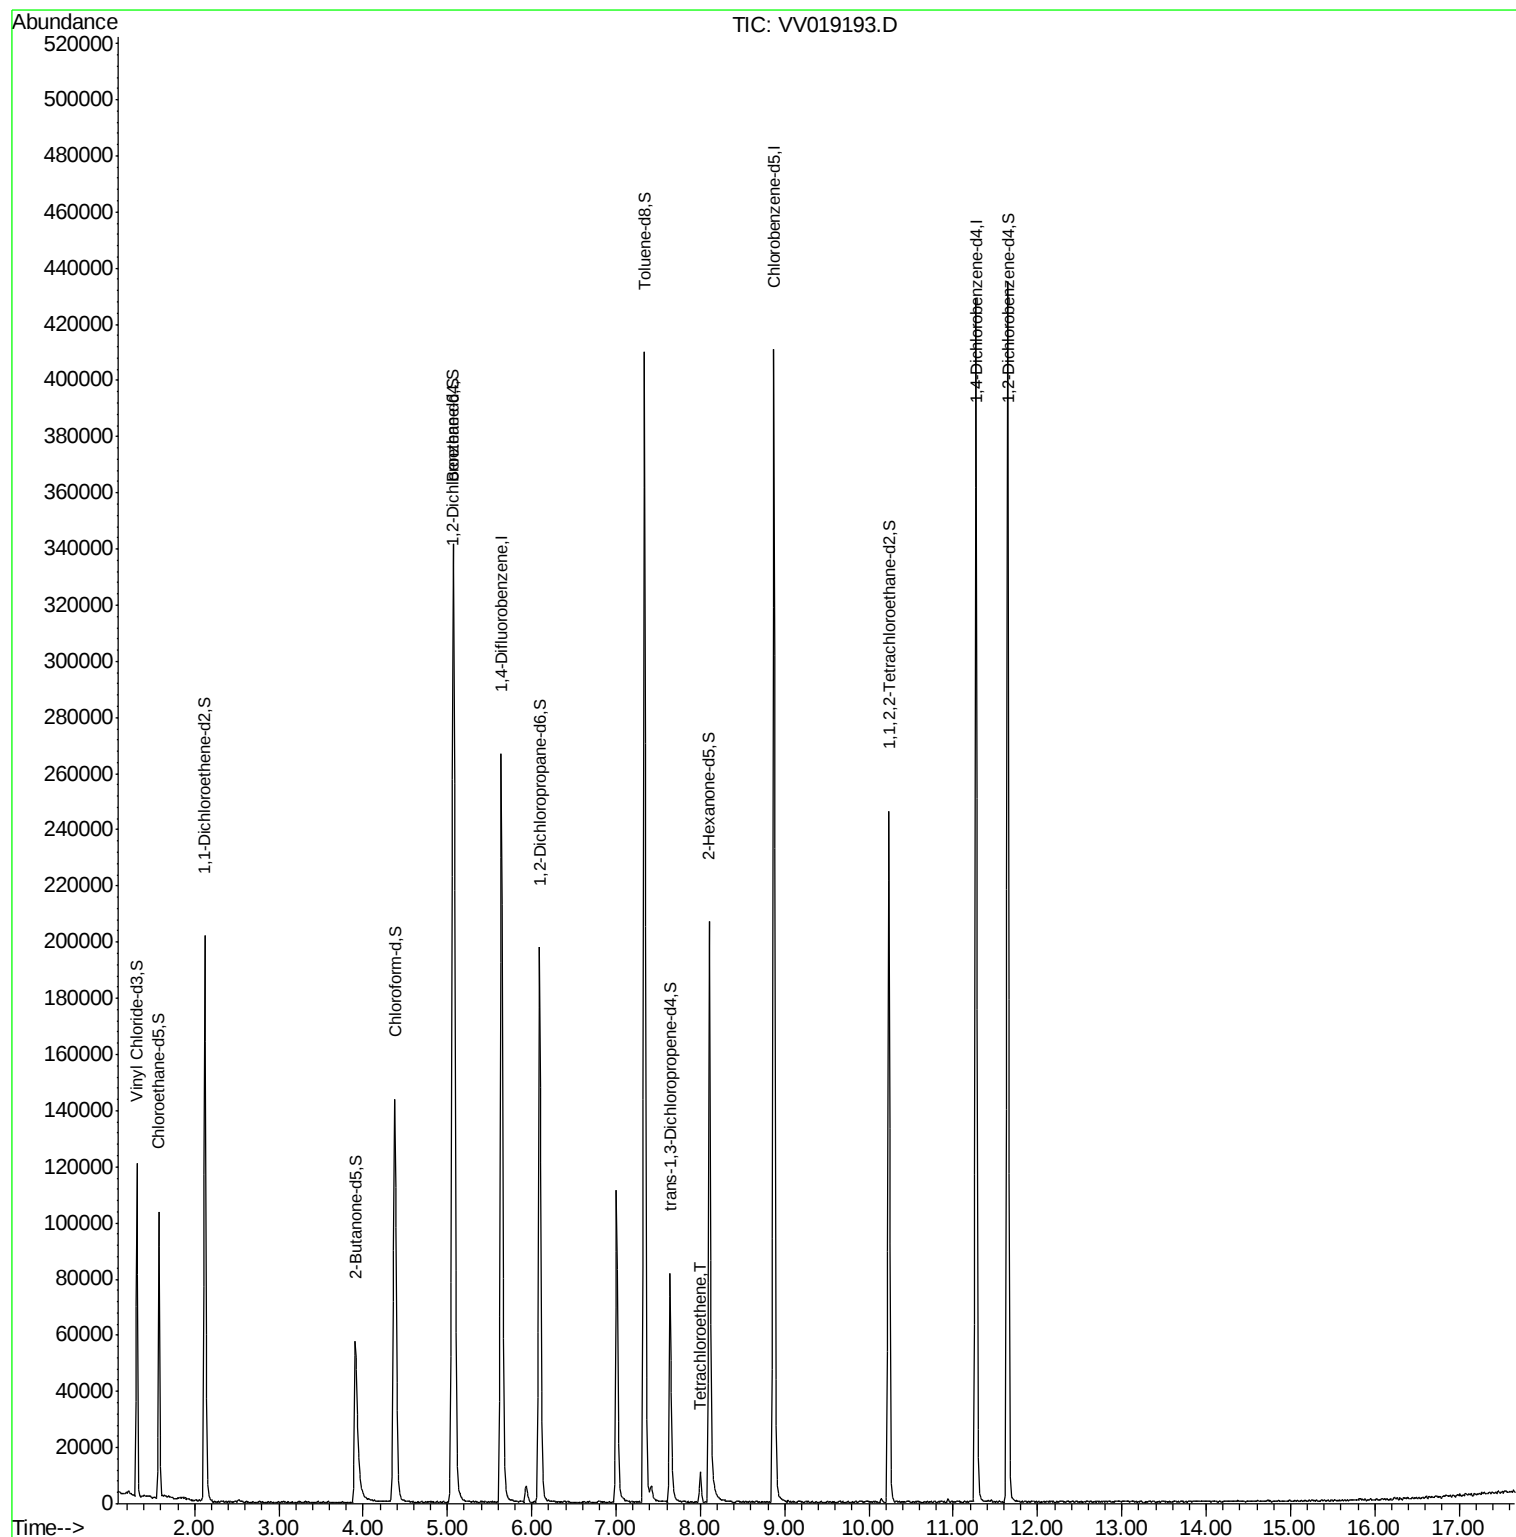

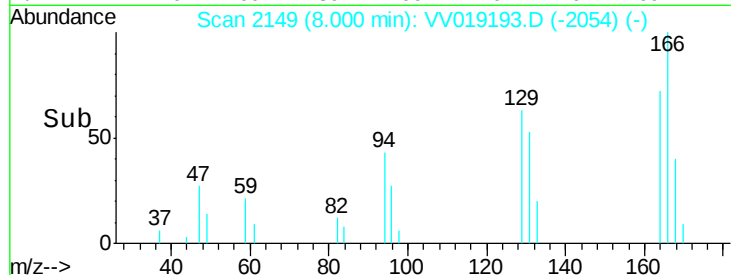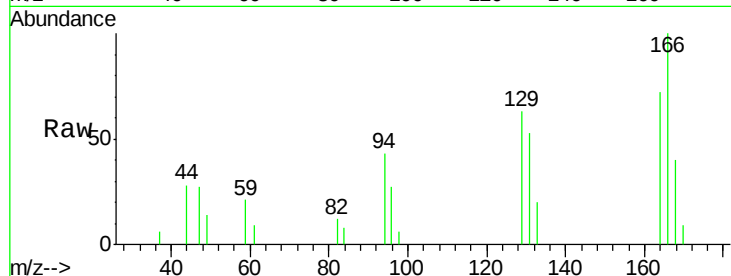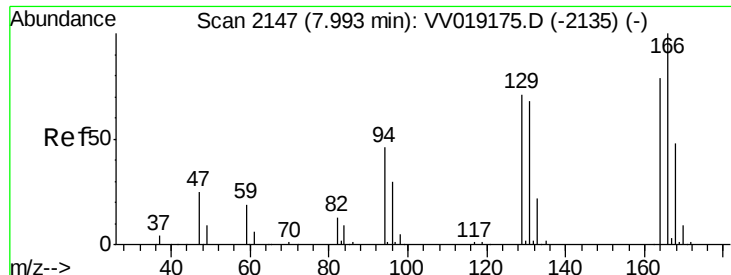

#46

Tetrachloroethene

Concen: 1.644 ug/L

RT: 8.00 min Scan# 2149

Delta R.T. 0.01 min

Lab File: VV019193.D

Acq: 30 Oct 2020 18:38

Instrument :

MSVOA_V

ClientSampleId :

VIBLK64

Tot Ion:164 Resp: 2401

Ion Ratio Lower Upper

164 100

129 87.9 63.2 117.4

131 74.6 60.3 112.1

166 139.7 88.3 163.9

Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

