

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV103020\
 Data File : VV019176.D
 Acq On : 30 Oct 2020 10:49
 Operator : SY/MD
 Sample : VV1030MBL01
 Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VV1030MBL01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	124246	125607	13.81%	1.983%
2	1.579	145	152	165	rVB	99345	113810	12.51%	1.797%
3	2.122	311	321	345	rVB	218522	324833	35.71%	5.129%
4	2.528	437	447	450	rBV3	809	1073	0.12%	0.017%
5	2.965	578	583	586	rVB2	403	380	0.04%	0.006%
6	2.987	586	590	595	rBV	164	235	0.03%	0.004%
7	3.122	629	632	636	rBV	276	272	0.03%	0.004%
8	3.293	682	685	688	rBV	214	180	0.02%	0.003%
9	3.447	730	733	737	rVB	284	246	0.03%	0.004%
10	3.781	831	837	840	rBV2	347	337	0.04%	0.005%
11	3.804	840	844	848	rVV	322	272	0.03%	0.004%
12	3.913	867	878	917	rBV	55954	170377	18.73%	2.690%
13	4.376	1006	1022	1054	rBV	147380	362845	39.89%	5.729%
14	4.582	1081	1086	1090	rBV3	383	413	0.05%	0.007%
15	4.614	1093	1096	1099	rVB3	284	190	0.02%	0.003%
16	4.634	1099	1102	1105	rBV2	310	244	0.03%	0.004%
17	4.685	1114	1118	1120	rBV2	289	208	0.02%	0.003%
18	4.698	1120	1122	1127	rVB2	359	300	0.03%	0.005%
19	4.733	1127	1133	1136	rBV2	381	449	0.05%	0.007%
20	4.778	1143	1147	1149	rBV2	262	195	0.02%	0.003%
21	4.852	1167	1170	1174	rVB	218	158	0.02%	0.002%
22	4.894	1180	1183	1186	rBV2	220	150	0.02%	0.002%
23	5.010	1216	1219	1221	rBV	212	161	0.02%	0.003%
24	5.071	1221	1238	1266	rBV2	353987	909599	100.00%	14.361%
25	5.412	1341	1344	1348	rBV3	329	341	0.04%	0.005%
26	5.476	1362	1364	1369	rBV	227	170	0.02%	0.003%
27	5.640	1404	1415	1448	rVV	187663	373259	41.04%	5.893%
28	5.894	1491	1494	1497	rBV	338	270	0.03%	0.004%
29	5.933	1497	1506	1520	rVB2	5793	11457	1.26%	0.181%
30	6.013	1529	1531	1536	rBV2	192	171	0.02%	0.003%
31	6.093	1543	1556	1578	rBV	201582	405232	44.55%	6.398%
32	6.228	1595	1598	1599	rBV	266	175	0.02%	0.003%
33	6.347	1628	1635	1636	rBV	352	294	0.03%	0.005%
34	6.399	1647	1651	1654	rBV2	232	224	0.02%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV103020\
 Data File : VV019176.D
 Acq On : 30 Oct 2020 10:49
 Operator : SY/MD
 Sample : VV1030MBL01
 Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VV1030MBL01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

35	6.441	1661	1664	1667	rBV2	271	208	0.02%	0.003%
36	6.482	1674	1677	1682	rBV2	252	241	0.03%	0.004%
37	6.508	1682	1685	1691	rVB2	260	290	0.03%	0.005%
38	6.717	1748	1750	1756	rVB	204	176	0.02%	0.003%
39	6.746	1756	1759	1761	rBV2	214	175	0.02%	0.003%
40	6.968	1823	1828	1830	rBV	289	164	0.02%	0.003%
41	7.006	1830	1840	1863	rBV	119834	214799	23.61%	3.391%
42	7.338	1930	1943	1961	rBV	426879	738465	81.19%	11.659%
43	7.585	2017	2020	2022	rBV2	308	166	0.02%	0.003%
44	7.601	2022	2025	2028	rVB	384	238	0.03%	0.004%
45	7.640	2028	2037	2067	rBV	86332	151072	16.61%	2.385%
46	7.839	2096	2099	2103	rVB	413	315	0.03%	0.005%
47	7.865	2103	2107	2110	rBV2	168	175	0.02%	0.003%
48	7.939	2128	2130	2133	rBV	282	194	0.02%	0.003%
49	8.006	2149	2151	2159	rVB3	432	327	0.04%	0.005%
50	8.042	2159	2162	2165	rBV2	294	214	0.02%	0.003%
51	8.058	2165	2167	2172	rVB	346	207	0.02%	0.003%
52	8.106	2172	2182	2211	rBV	206563	368674	40.53%	5.821%
53	8.482	2295	2299	2302	rBV2	481	390	0.04%	0.006%
54	8.511	2306	2308	2311	rVV	265	167	0.02%	0.003%
55	8.569	2324	2326	2328	rBV	346	211	0.02%	0.003%
56	8.678	2354	2360	2362	rBV2	362	278	0.03%	0.004%
57	8.711	2366	2370	2371	rBV	194	156	0.02%	0.002%
58	8.871	2409	2420	2449	rBV	291088	475747	52.30%	7.511%
59	9.100	2487	2491	2492	rBV2	350	215	0.02%	0.003%
60	9.167	2506	2512	2517	rBV3	655	816	0.09%	0.013%
61	9.206	2521	2524	2533	rBV2	298	424	0.05%	0.007%
62	9.415	2583	2589	2593	rBV	260	287	0.03%	0.005%
63	9.495	2611	2614	2619	rBV	123	149	0.02%	0.002%
64	9.920	2741	2746	2750	rVB	384	446	0.05%	0.007%
65	9.958	2756	2758	2761	rVB	306	161	0.02%	0.003%
66	9.993	2765	2769	2773	rBV2	253	277	0.03%	0.004%
67	10.042	2781	2784	2789	rVB	375	337	0.04%	0.005%
68	10.074	2791	2794	2801	rVB2	291	304	0.03%	0.005%
69	10.148	2806	2817	2824	rBV3	1850	2811	0.31%	0.044%
70	10.235	2832	2844	2860	rBV	251462	394413	43.36%	6.227%
71	10.363	2880	2884	2887	rBV3	500	463	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV103020\
 Data File : VV019176.D
 Acq On : 30 Oct 2020 10:49
 Operator : SY/MD
 Sample : VV1030MBL01
 Misc : 5.0µ/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VV1030MBL01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

72	10.411	2896	2899	2901	rBV	293	185	0.02%	0.003%
73	10.559	2942	2945	2946	rBV	296	164	0.02%	0.003%
74	10.604	2956	2959	2962	rBV	286	209	0.02%	0.003%
75	10.685	2981	2984	2986	rBV2	266	176	0.02%	0.003%
76	10.865	3038	3040	3044	rVB	334	215	0.02%	0.003%
77	10.910	3050	3054	3056	rBV	224	166	0.02%	0.003%
78	10.936	3058	3062	3071	rVB5	1569	1978	0.22%	0.031%
79	11.051	3095	3098	3104	rBV2	335	408	0.04%	0.006%
80	11.167	3129	3134	3138	rBV3	440	519	0.06%	0.008%
81	11.206	3144	3146	3149	rVB3	464	259	0.03%	0.004%
82	11.270	3154	3166	3186	rBV	298200	459535	50.52%	7.255%
83	11.408	3206	3209	3212	rBV3	741	510	0.06%	0.008%
84	11.646	3271	3283	3307	rBV	451550	706372	77.66%	11.153%
85	11.733	3307	3310	3314	rBV	612	445	0.05%	0.007%
86	11.800	3328	3331	3339	rVB2	438	531	0.06%	0.008%
87	11.842	3340	3344	3346	rVB	357	226	0.02%	0.004%
88	11.881	3349	3356	3359	rBV2	352	374	0.04%	0.006%
89	11.948	3375	3377	3380	rBV	343	186	0.02%	0.003%
90	12.257	3470	3473	3479	rVB	309	276	0.03%	0.004%
91	12.312	3487	3490	3493	rBV2	246	155	0.02%	0.002%
92	12.344	3497	3500	3503	rBV2	281	250	0.03%	0.004%
93	12.759	3626	3629	3630	rBV	267	159	0.02%	0.003%
94	13.061	3721	3723	3728	rVB2	276	223	0.02%	0.004%
95	13.106	3733	3737	3743	rBV2	345	401	0.04%	0.006%
96	13.238	3775	3778	3780	rBV	264	204	0.02%	0.003%
97	13.508	3858	3862	3864	rVB	335	251	0.03%	0.004%
98	13.598	3885	3890	3893	rBV2	308	343	0.04%	0.005%
99	13.672	3910	3913	3918	rBV2	285	300	0.03%	0.005%
100	14.279	4098	4102	4105	rBV2	406	378	0.04%	0.006%


Sum of corrected areas: 6333677

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV103020\
Data File : VV019176.D
Acq On : 30 Oct 2020 10:49
Operator : SY/MD
Sample : VV1030MBL01
Misc : 5.0µL/100µL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VV1030MBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

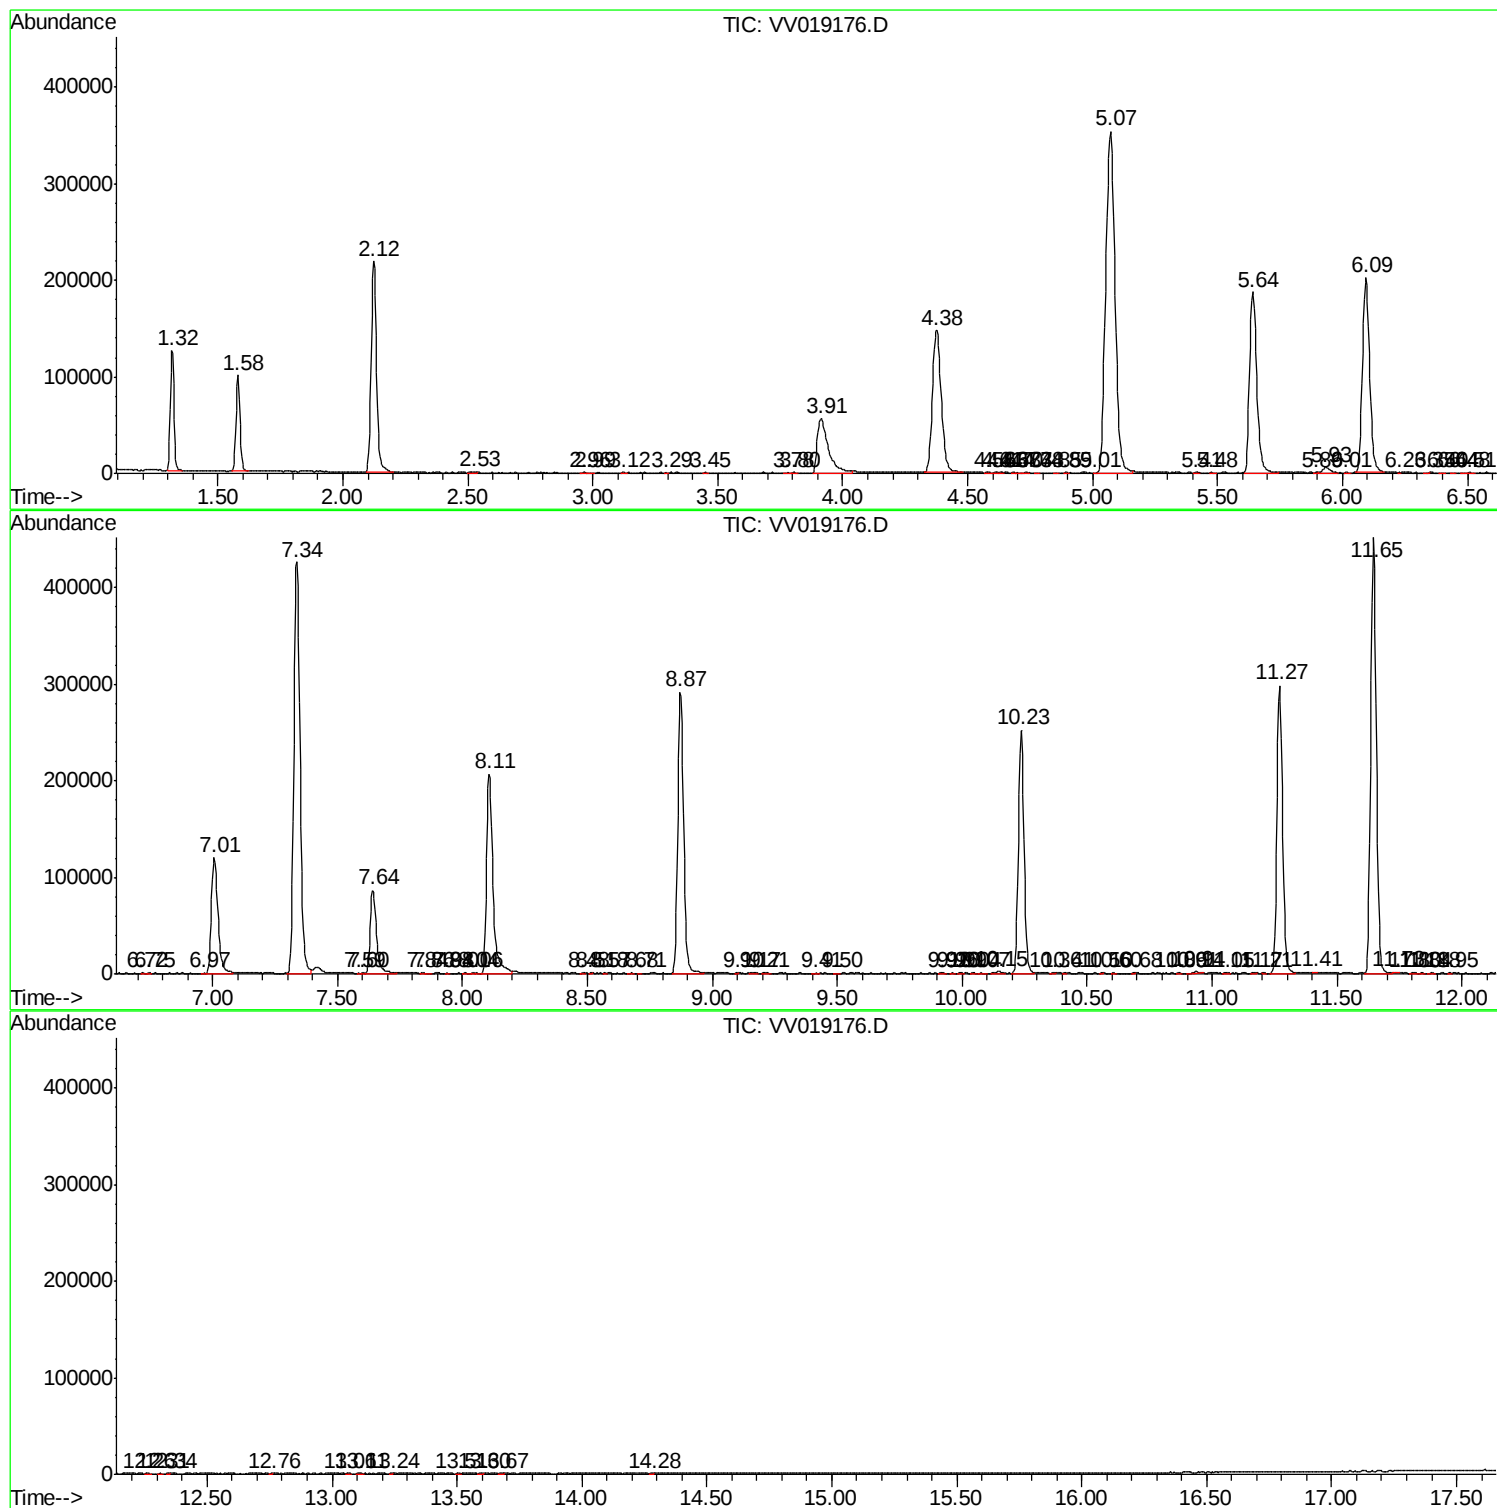

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV103020\
Data File : VV019176.D
Acq On : 30 Oct 2020 10:49
Operator : SY/MD
Sample : VV1030MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VV1030MBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV103020\
Data File : VV019176.D
Acq On : 30 Oct 2020 10:49
Operator : SY/MD
Sample : VV1030MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VV1030MBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc