

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV103020\
 Data File : VV019180.D
 Acq On : 30 Oct 2020 13:29
 Operator : SY/MD
 Sample : L4502-20ME 2X
 Misc : 6.07g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG443ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	86	rVB	211655	229910	13.69%	1.810%
2	1.579	144	152	164	rBV	176268	215112	12.81%	1.694%
3	2.113	307	318	350	rBV	402848	593880	35.36%	4.676%
4	2.360	392	395	396	rBV2	280	163	0.01%	0.001%
5	2.460	419	426	429	rBV2	449	639	0.04%	0.005%
6	2.521	441	445	452	rVB3	1431	1739	0.10%	0.014%
7	2.698	497	500	504	rVB2	453	289	0.02%	0.002%
8	2.753	513	517	520	rBV3	576	413	0.02%	0.003%
9	2.868	550	553	556	rVB2	277	174	0.01%	0.001%
10	2.897	556	562	563	rBV2	364	287	0.02%	0.002%
11	3.122	629	632	635	rBV	297	205	0.01%	0.002%
12	3.142	635	638	641	rVB	223	131	0.01%	0.001%
13	3.296	683	686	693	rVB2	320	358	0.02%	0.003%
14	3.386	711	714	717	rBV	234	150	0.01%	0.001%
15	3.402	717	719	721	rVB	269	126	0.01%	0.001%
16	3.425	721	726	729	rBV2	332	368	0.02%	0.003%
17	3.698	808	811	814	rVV	294	173	0.01%	0.001%
18	3.856	857	860	866	rBV	113	122	0.01%	0.001%
19	3.913	866	878	930	rBV	85589	311701	18.56%	2.454%
20	4.370	1004	1020	1049	rBV	272366	667916	39.77%	5.259%
21	4.650	1105	1107	1109	rBV2	307	199	0.01%	0.002%
22	4.884	1175	1180	1183	rBV2	263	247	0.01%	0.002%
23	5.064	1218	1236	1261	rBV2	664407	1679509	100.00%	13.224%
24	5.405	1340	1342	1343	rBV	299	150	0.01%	0.001%
25	5.470	1361	1362	1369	rVV2	177	133	0.01%	0.001%
26	5.637	1402	1414	1442	rBV	356374	704967	41.97%	5.551%
27	5.929	1494	1505	1525	rVB6	14140	31656	1.88%	0.249%
28	6.007	1526	1529	1532	rBV4	742	564	0.03%	0.004%
29	6.090	1541	1555	1578	rBV	369787	749010	44.60%	5.898%
30	6.302	1617	1621	1629	rBV3	362	451	0.03%	0.004%
31	6.383	1643	1646	1648	rBV	204	158	0.01%	0.001%
32	6.489	1677	1679	1683	rVB2	274	141	0.01%	0.001%
33	6.540	1689	1695	1699	rBV3	451	542	0.03%	0.004%
34	6.576	1704	1706	1713	rVB2	307	262	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV103020\
 Data File : VV019180.D
 Acq On : 30 Oct 2020 13:29
 Operator : SY/MD
 Sample : L4502-20ME 2X
 Misc : 6.07g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG443ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

35	6.611	1713	1717	1720	rBV2	334	257	0.02%	0.002%
36	6.659	1729	1732	1735	rBV2	315	204	0.01%	0.002%
37	6.679	1736	1738	1743	rVB2	490	322	0.02%	0.003%
38	6.727	1748	1753	1757	rBV2	330	335	0.02%	0.003%
39	6.765	1762	1765	1768	rBV	267	146	0.01%	0.001%
40	6.781	1768	1770	1773	rBV2	253	147	0.01%	0.001%
41	6.836	1785	1787	1789	rBV	264	133	0.01%	0.001%
42	7.003	1827	1839	1861	rBV	228830	407760	24.28%	3.211%
43	7.196	1896	1899	1901	rBV	329	225	0.01%	0.002%
44	7.335	1927	1942	1960	rBV	808655	1384378	82.43%	10.900%
45	7.640	2026	2037	2066	rBV	163807	286483	17.06%	2.256%
46	7.994	2135	2147	2168	rBV	413656	679004	40.43%	5.346%
47	8.116	2173	2185	2221	rBV	269425	742467	44.21%	5.846%
48	8.379	2265	2267	2270	rBV2	361	252	0.02%	0.002%
49	8.511	2306	2308	2310	rVB2	405	189	0.01%	0.001%
50	8.627	2340	2344	2345	rBV	319	192	0.01%	0.002%
51	8.672	2355	2358	2361	rVB2	237	151	0.01%	0.001%
52	8.749	2379	2382	2385	rVB2	292	174	0.01%	0.001%
53	8.769	2385	2388	2389	rBV	278	170	0.01%	0.001%
54	8.871	2408	2420	2445	rBV	545684	889581	52.97%	7.004%
55	9.074	2482	2483	2488	rVB	386	239	0.01%	0.002%
56	9.106	2488	2493	2497	rVB2	358	359	0.02%	0.003%
57	9.129	2497	2500	2505	rBV2	211	188	0.01%	0.001%
58	9.164	2505	2511	2513	rBV2	813	820	0.05%	0.006%
59	9.235	2531	2533	2537	rBV2	252	240	0.01%	0.002%
60	9.280	2545	2547	2552	rVB2	245	168	0.01%	0.001%
61	9.412	2585	2588	2590	rBV2	336	231	0.01%	0.002%
62	9.489	2608	2612	2615	rVB	234	200	0.01%	0.002%
63	9.714	2678	2682	2685	rBV2	307	250	0.01%	0.002%
64	9.743	2688	2691	2694	rVV	169	122	0.01%	0.001%
65	9.762	2694	2697	2700	rVV	229	136	0.01%	0.001%
66	9.791	2703	2706	2709	rVB	307	181	0.01%	0.001%
67	9.842	2719	2722	2726	rBV2	332	322	0.02%	0.003%
68	9.878	2730	2733	2735	rBV	256	171	0.01%	0.001%
69	9.997	2765	2770	2771	rBV	199	171	0.01%	0.001%
70	10.006	2771	2773	2779	rVB2	330	298	0.02%	0.002%
71	10.039	2779	2783	2785	rBV2	327	254	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV103020\
 Data File : VV019180.D
 Acq On : 30 Oct 2020 13:29
 Operator : SY/MD
 Sample : L4502-20ME 2X
 Misc : 6.07g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG443ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

72	10.055	2785	2788	2794	rVB	277	289	0.02%	0.002%
73	10.145	2809	2816	2824	rBV4	2626	3811	0.23%	0.030%
74	10.241	2833	2846	2861	rBV	464646	761479	45.34%	5.996%
75	10.434	2902	2906	2910	rBV	242	261	0.02%	0.002%
76	10.572	2945	2949	2951	rBV2	310	276	0.02%	0.002%
77	10.585	2951	2953	2955	rBV3	495	299	0.02%	0.002%
78	10.723	2993	2996	2999	rBV2	309	224	0.01%	0.002%
79	10.775	3008	3012	3014	rBV	282	248	0.01%	0.002%
80	10.810	3020	3023	3026	rBV2	360	306	0.02%	0.002%
81	10.855	3036	3037	3040	rVB	350	147	0.01%	0.001%
82	10.936	3056	3062	3071	rBV8	2318	3220	0.19%	0.025%
83	11.119	3116	3119	3122	rBV	311	213	0.01%	0.002%
84	11.164	3126	3133	3143	rBV2	1239	1696	0.10%	0.013%
85	11.270	3150	3166	3189	rBV	604749	937473	55.82%	7.381%
86	11.649	3271	3284	3303	rVV	893496	1398122	83.25%	11.008%
87	11.788	3324	3327	3328	rBV	413	205	0.01%	0.002%
88	11.852	3345	3347	3349	rBV2	336	151	0.01%	0.001%
89	11.871	3349	3353	3357	rVB3	516	447	0.03%	0.004%
90	11.913	3364	3366	3370	rVB2	316	197	0.01%	0.002%
91	12.466	3535	3538	3544	rVB	353	344	0.02%	0.003%
92	12.495	3544	3547	3548	rBV2	278	169	0.01%	0.001%
93	12.749	3623	3626	3627	rBV	233	129	0.01%	0.001%
94	13.080	3723	3729	3733	rBV2	332	408	0.02%	0.003%
95	13.145	3746	3749	3755	rVB2	310	272	0.02%	0.002%
96	13.173	3755	3758	3761	rBV	348	313	0.02%	0.002%
97	13.296	3793	3796	3800	rBV2	451	346	0.02%	0.003%
98	13.556	3874	3877	3881	rBV2	246	250	0.01%	0.002%
99	14.096	4043	4045	4048	rBV	215	122	0.01%	0.001%
100	14.694	4227	4231	4232	rBV	313	241	0.01%	0.002%


Sum of corrected areas: 12700423

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV103020\
Data File : VV019180.D
Acq On : 30 Oct 2020 13:29
Operator : SY/MD
Sample : L4502-20ME 2X
Misc : 6.07g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG443ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

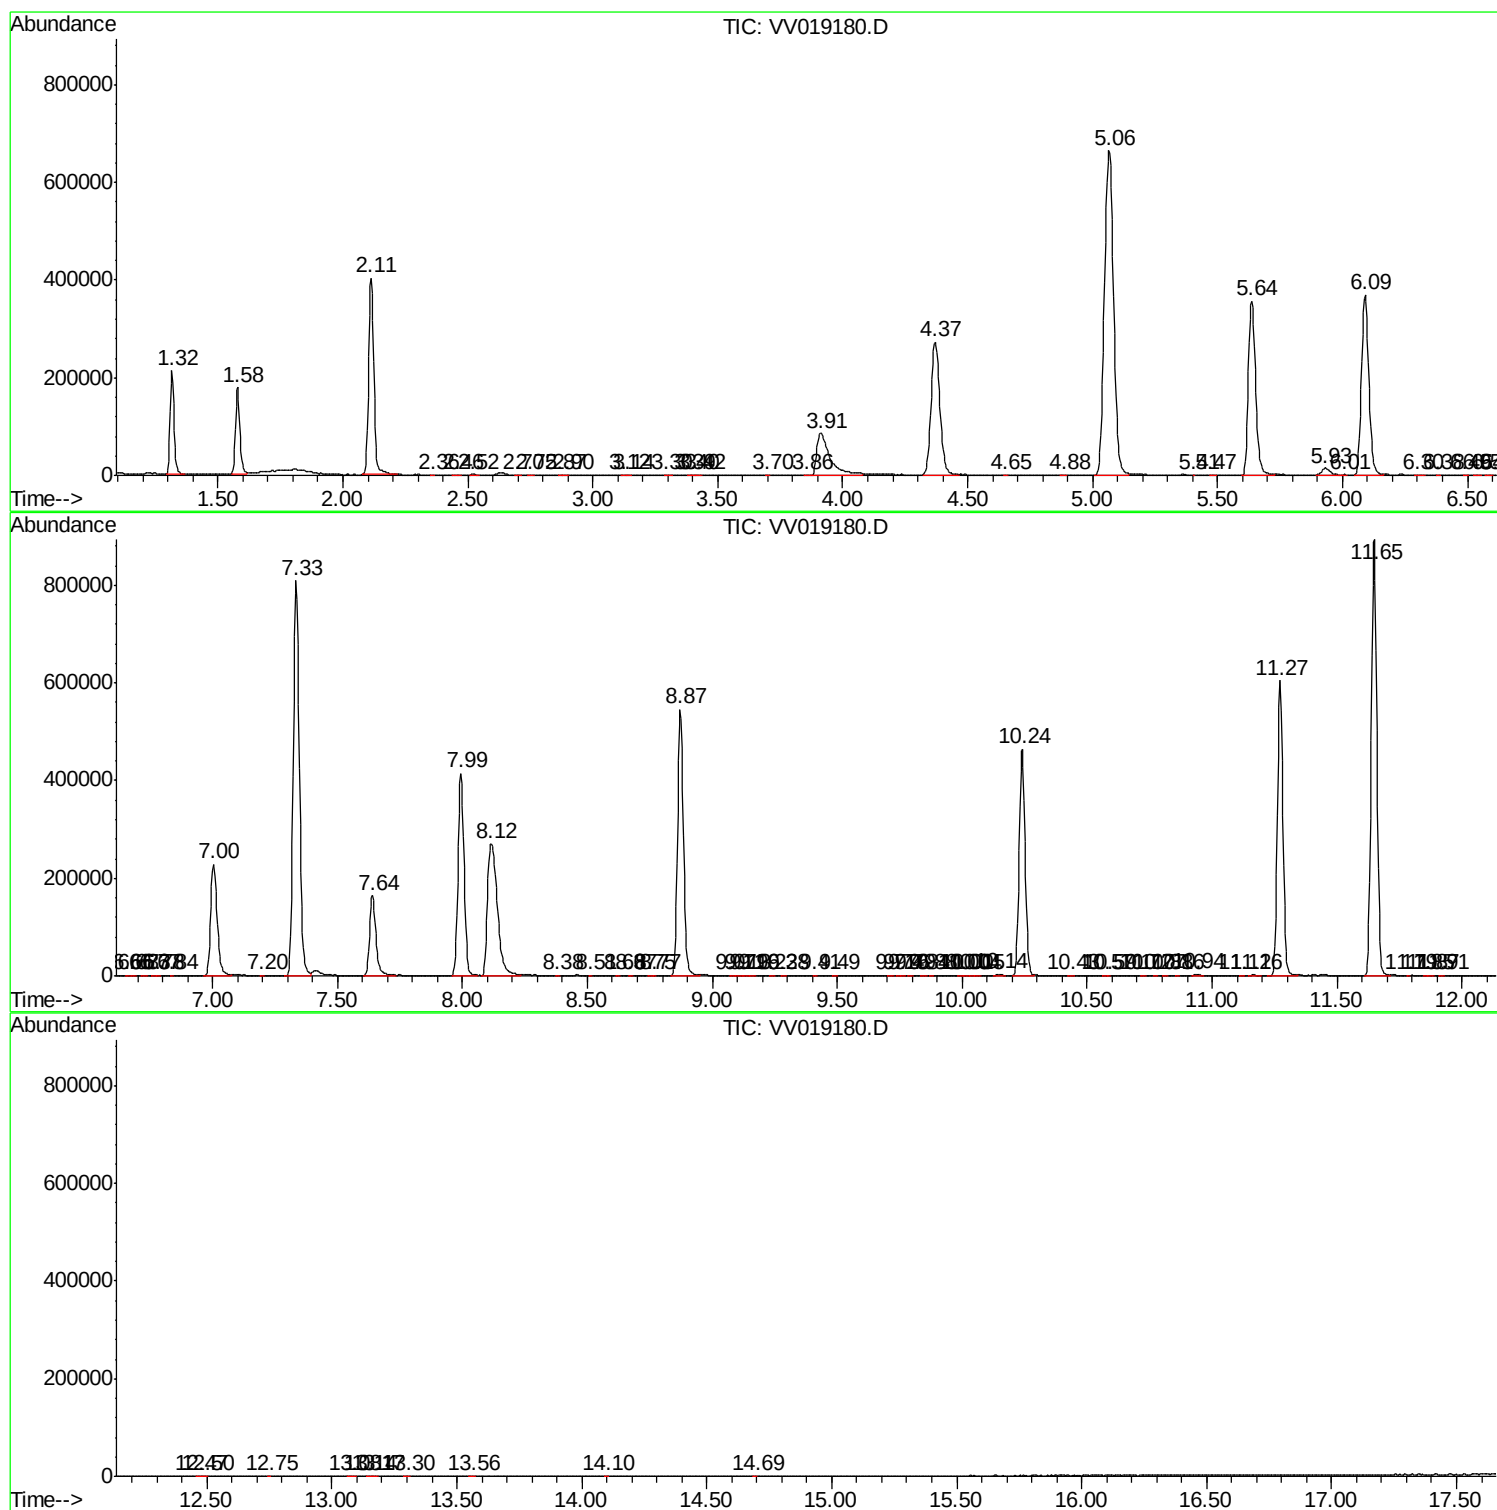

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV103020\
Data File : VV019180.D
Acq On : 30 Oct 2020 13:29
Operator : SY/MD
Sample : L4502-20ME 2X
Misc : 6.07g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG443ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV103020\
Data File : VV019180.D
Acq On : 30 Oct 2020 13:29
Operator : SY/MD
Sample : L4502-20ME 2X
Misc : 6.07g/5.0mL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG443ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc