

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV103020\
 Data File : VV019182.D
 Acq On : 30 Oct 2020 14:16
 Operator : SY/MD
 Sample : L4502-22ME
 Misc : 5.27g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG445ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	89	rVB	218341	267915	13.46%	2.093%
2	1.579	144	152	170	rBV	149161	252572	12.69%	1.973%
3	2.103	304	315	327	rBV	468984	675981	33.97%	5.280%
4	2.380	398	401	404	rVB2	337	189	0.01%	0.001%
5	2.553	451	455	458	rBV2	354	326	0.02%	0.003%
6	2.582	461	464	467	rBV	372	215	0.01%	0.002%
7	2.631	467	479	496	rVV	6683	14462	0.73%	0.113%
8	2.888	556	559	562	rBV2	293	176	0.01%	0.001%
9	3.068	612	615	617	rBV	282	174	0.01%	0.001%
10	3.135	633	636	640	rVB	240	203	0.01%	0.002%
11	3.174	645	648	651	rBV2	272	240	0.01%	0.002%
12	3.229	663	665	668	rBV	200	154	0.01%	0.001%
13	3.364	705	707	711	rVV2	339	235	0.01%	0.002%
14	3.717	814	817	820	rBV	219	169	0.01%	0.001%
15	3.920	868	880	931	rBV2	83856	345993	17.39%	2.702%
16	4.370	1005	1020	1061	rVB	310546	788588	39.63%	6.159%
17	4.579	1081	1085	1088	rBV3	373	341	0.02%	0.003%
18	4.630	1099	1101	1106	rBV2	221	202	0.01%	0.002%
19	4.711	1123	1126	1128	rBV	248	149	0.01%	0.001%
20	4.859	1168	1172	1176	rBV	421	313	0.02%	0.002%
21	4.949	1195	1200	1203	rBV	272	233	0.01%	0.002%
22	5.065	1219	1236	1277	rBV2	805218	1990103	100.00%	15.544%
23	5.357	1320	1327	1335	rBV6	1414	2593	0.13%	0.020%
24	5.489	1364	1368	1370	rBV2	435	323	0.02%	0.003%
25	5.589	1395	1399	1403	rBV2	239	245	0.01%	0.002%
26	5.637	1403	1414	1452	rVV	185194	386082	19.40%	3.016%
27	5.888	1488	1492	1494	rBV2	247	198	0.01%	0.002%
28	5.926	1494	1504	1524	rVB6	12834	28389	1.43%	0.222%
29	6.010	1524	1530	1532	rBV2	1336	1361	0.07%	0.011%
30	6.090	1540	1555	1589	rBV	418383	876924	44.06%	6.849%
31	6.437	1657	1663	1668	rBV2	304	337	0.02%	0.003%
32	6.492	1677	1680	1683	rBV2	258	214	0.01%	0.002%
33	6.534	1690	1693	1697	rBV2	295	248	0.01%	0.002%
34	6.592	1707	1711	1713	rBV2	294	211	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV103020\
 Data File : VV019182.D
 Acq On : 30 Oct 2020 14:16
 Operator : SY/MD
 Sample : L4502-22ME
 Misc : 5.27g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG445ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

35	6.634	1720	1724	1727	rBV2	272	243	0.01%	0.002%
36	6.653	1727	1730	1731	rBV	318	182	0.01%	0.001%
37	6.804	1773	1777	1779	rBV2	268	258	0.01%	0.002%
38	6.852	1789	1792	1796	rBV	256	262	0.01%	0.002%
39	7.007	1828	1840	1874	rBV	250642	487563	24.50%	3.808%
40	7.248	1912	1915	1918	rBV3	416	246	0.01%	0.002%
41	7.335	1929	1942	1960	rBV	923167	1628096	81.81%	12.716%
42	7.640	2026	2037	2070	rBV	167712	342392	17.20%	2.674%
43	7.868	2104	2108	2113	rBV4	440	513	0.03%	0.004%
44	7.917	2119	2123	2125	rBV2	284	167	0.01%	0.001%
45	7.994	2136	2147	2171	rVB	234171	395529	19.87%	3.089%
46	8.138	2174	2192	2228	rBV	258217	870562	43.74%	6.800%
47	8.640	2345	2348	2350	rVB	350	198	0.01%	0.002%
48	8.656	2350	2353	2356	rBV	345	192	0.01%	0.001%
49	8.682	2358	2361	2364	rVV	398	195	0.01%	0.002%
50	8.701	2364	2367	2374	rVB	273	246	0.01%	0.002%
51	8.730	2374	2376	2378	rBV2	319	191	0.01%	0.001%
52	8.756	2381	2384	2387	rVB	312	215	0.01%	0.002%
53	8.775	2387	2390	2393	rBV	322	194	0.01%	0.002%
54	8.875	2409	2421	2441	rBV	271047	496450	24.95%	3.878%
55	9.042	2468	2473	2475	rBV3	349	327	0.02%	0.003%
56	9.129	2494	2500	2502	rBV	293	283	0.01%	0.002%
57	9.171	2507	2513	2515	rBV2	748	758	0.04%	0.006%
58	9.396	2581	2583	2586	rBV2	204	166	0.01%	0.001%
59	9.518	2614	2621	2626	rBV2	317	377	0.02%	0.003%
60	9.582	2636	2641	2647	rVB2	534	719	0.04%	0.006%
61	9.621	2647	2653	2657	rBV2	210	258	0.01%	0.002%
62	9.836	2716	2720	2724	rBV2	179	203	0.01%	0.002%
63	9.907	2738	2742	2745	rBV2	221	262	0.01%	0.002%
64	9.942	2750	2753	2755	rBV2	230	163	0.01%	0.001%
65	9.978	2760	2764	2766	rBV	235	168	0.01%	0.001%
66	10.023	2775	2778	2783	rVB2	246	253	0.01%	0.002%
67	10.077	2791	2795	2798	rBV2	199	164	0.01%	0.001%
68	10.148	2808	2817	2826	rVB3	3209	5068	0.25%	0.040%
69	10.244	2833	2847	2864	rBV	502602	873358	43.89%	6.821%
70	10.367	2882	2885	2887	rBV3	696	474	0.02%	0.004%
71	10.476	2916	2919	2922	rBV	378	330	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV103020\
 Data File : VV019182.D
 Acq On : 30 Oct 2020 14:16
 Operator : SY/MD
 Sample : L4502-22ME
 Misc : 5.27g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG445ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

72	10.563	2942	2946	2947	rBV2	358	227	0.01%	0.002%
73	10.669	2977	2979	2982	rBV2	316	179	0.01%	0.001%
74	10.707	2988	2991	2994	rBV	299	167	0.01%	0.001%
75	10.765	3006	3009	3012	rBV2	201	170	0.01%	0.001%
76	10.862	3036	3039	3043	rBV	241	220	0.01%	0.002%
77	10.936	3055	3062	3076	rVB7	3058	5106	0.26%	0.040%
78	10.990	3076	3079	3082	rVB2	251	199	0.01%	0.002%
79	11.006	3082	3084	3088	rBV2	263	204	0.01%	0.002%
80	11.029	3088	3091	3096	rBV	295	246	0.01%	0.002%
81	11.093	3107	3111	3113	rBV	359	299	0.02%	0.002%
82	11.164	3128	3133	3144	rBV4	1575	2306	0.12%	0.018%
83	11.273	3156	3167	3185	rBV	313630	485479	24.39%	3.792%
84	11.405	3202	3208	3210	rBV3	1037	1130	0.06%	0.009%
85	11.489	3229	3234	3237	rBV2	518	419	0.02%	0.003%
86	11.650	3272	3284	3307	rBV	989961	1559248	78.35%	12.179%
87	11.772	3319	3322	3327	rBV2	545	547	0.03%	0.004%
88	12.071	3413	3415	3420	rVB2	375	214	0.01%	0.002%
89	12.109	3425	3427	3431	rVB2	310	189	0.01%	0.001%
90	12.479	3539	3542	3545	rBV	301	247	0.01%	0.002%
91	12.662	3594	3599	3600	rBV	172	165	0.01%	0.001%
92	12.730	3617	3620	3622	rBV	267	186	0.01%	0.001%
93	12.778	3632	3635	3638	rBV	316	255	0.01%	0.002%
94	12.849	3653	3657	3659	rBV	252	225	0.01%	0.002%
95	13.145	3746	3749	3754	rBV2	221	242	0.01%	0.002%
96	13.916	3984	3989	3993	rBV2	446	551	0.03%	0.004%
97	14.116	4048	4051	4053	rBV2	352	239	0.01%	0.002%
98	14.164	4060	4066	4073	rBV3	390	636	0.03%	0.005%
99	14.379	4131	4133	4135	rBV2	346	229	0.01%	0.002%
100	14.971	4314	4317	4319	rBV3	381	308	0.02%	0.002%


Sum of corrected areas: 12803115

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV103020\
Data File : VV019182.D
Acq On : 30 Oct 2020 14:16
Operator : SY/MD
Sample : L4502-22ME
Misc : 5.27g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG445ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

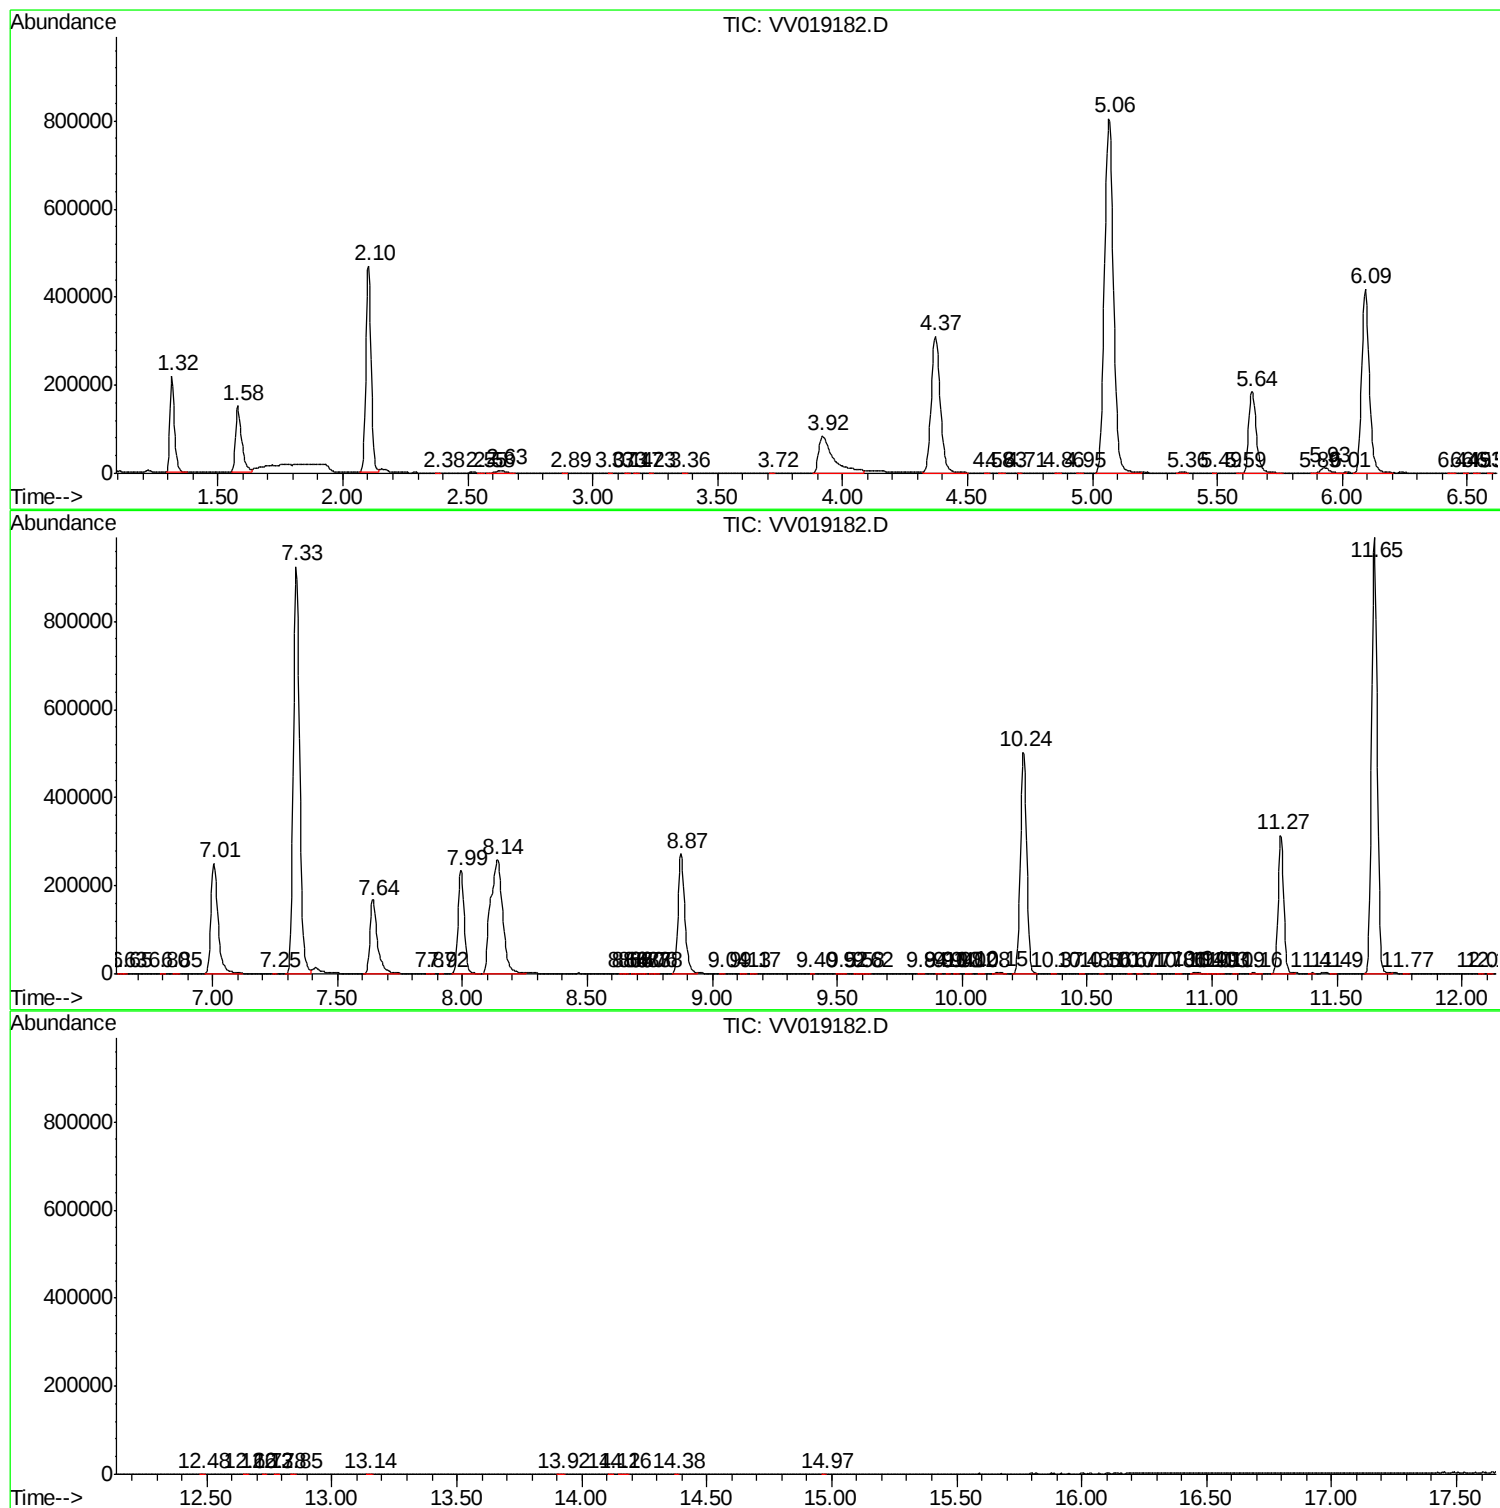

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV103020\
Data File : VV019182.D
Acq On : 30 Oct 2020 14:16
Operator : SY/MD
Sample : L4502-22ME
Misc : 5.27g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG445ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV103020\
Data File : VV019182.D
Acq On : 30 Oct 2020 14:16
Operator : SY/MD
Sample : L4502-22ME
Misc : 5.27g/5.0mL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG445ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc