

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV103020\
 Data File : VV019190.D
 Acq On : 30 Oct 2020 17:26
 Operator : SY/MD
 Sample : L4543-01DL 1000X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG455DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	84	rVB	142174	137394	14.27%	1.735%
2	1.579	144	152	169	rBV	115138	129986	13.50%	1.641%
3	2.122	311	321	340	rBV	227083	335146	34.81%	4.232%
4	2.341	387	389	391	rBV	243	169	0.02%	0.002%
5	2.392	400	405	409	rBV2	306	299	0.03%	0.004%
6	2.527	440	447	454	rVB4	835	1207	0.13%	0.015%
7	2.679	490	494	497	rBV2	311	308	0.03%	0.004%
8	2.974	577	586	597	rBV	523	1049	0.11%	0.013%
9	3.109	625	628	630	rBV	185	140	0.01%	0.002%
10	3.126	630	633	637	rVV2	209	167	0.02%	0.002%
11	3.283	679	682	685	rVB2	232	147	0.02%	0.002%
12	3.421	722	725	729	rVV2	186	176	0.02%	0.002%
13	3.479	740	743	746	rBV2	203	179	0.02%	0.002%
14	3.589	774	777	781	rVB	193	139	0.01%	0.002%
15	3.675	800	804	808	rVV	211	192	0.02%	0.002%
16	3.704	810	813	818	rVB	411	306	0.03%	0.004%
17	3.762	827	831	833	rBV	122	124	0.01%	0.002%
18	3.839	851	855	857	rBV2	239	156	0.02%	0.002%
19	3.907	864	876	916	rBV2	65014	189789	19.71%	2.397%
20	4.376	1006	1022	1050	rBV	156441	385651	40.05%	4.870%
21	4.569	1080	1082	1083	rBV	304	134	0.01%	0.002%
22	4.630	1098	1101	1103	rBV	268	164	0.02%	0.002%
23	4.672	1111	1114	1121	rVB2	408	315	0.03%	0.004%
24	4.704	1121	1124	1127	rVB2	289	149	0.02%	0.002%
25	4.736	1127	1134	1136	rBV2	225	239	0.02%	0.003%
26	4.939	1195	1197	1199	rBV	266	135	0.01%	0.002%
27	4.987	1210	1212	1218	rBV2	218	216	0.02%	0.003%
28	5.071	1221	1238	1265	rBV2	374159	962903	100.00%	12.160%
29	5.244	1290	1292	1293	rBV	389	147	0.02%	0.002%
30	5.344	1322	1323	1327	rBV2	381	257	0.03%	0.003%
31	5.402	1338	1341	1346	rBV2	392	396	0.04%	0.005%
32	5.424	1346	1348	1351	rBV	209	146	0.02%	0.002%
33	5.534	1379	1382	1386	rBV	335	277	0.03%	0.003%
34	5.640	1403	1415	1448	rVV	275072	548463	56.96%	6.926%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV103020\
 Data File : VV019190.D
 Acq On : 30 Oct 2020 17:26
 Operator : SY/MD
 Sample : L4543-01DL 1000X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG455DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

35	5.939	1496	1508	1529	rVB4	20289	46541	4.83%	0.588%
36	6.093	1543	1556	1581	rVV	215602	434490	45.12%	5.487%
37	6.305	1619	1622	1624	rVB	222	147	0.02%	0.002%
38	6.331	1625	1630	1633	rBV2	228	268	0.03%	0.003%
39	6.373	1637	1643	1648	rBV2	294	349	0.04%	0.004%
40	6.514	1684	1687	1690	rBV2	175	124	0.01%	0.002%
41	7.006	1829	1840	1866	rBV	122530	221491	23.00%	2.797%
42	7.222	1905	1907	1911	rBV2	252	154	0.02%	0.002%
43	7.270	1919	1922	1924	rBV2	343	241	0.03%	0.003%
44	7.338	1931	1943	1962	rBV	439724	754981	78.41%	9.534%
45	7.643	2028	2038	2058	rBV	88862	154088	16.00%	1.946%
46	7.813	2088	2091	2092	rBV	300	144	0.01%	0.002%
47	7.846	2099	2101	2103	rBV	316	171	0.02%	0.002%
48	7.997	2135	2148	2169	rBV	419638	703576	73.07%	8.885%
49	8.106	2173	2182	2214	rBV	234390	405994	42.16%	5.127%
50	8.453	2284	2290	2294	rBV3	463	431	0.04%	0.005%
51	8.720	2371	2373	2375	rBV2	218	126	0.01%	0.002%
52	8.759	2378	2385	2389	rBV2	308	421	0.04%	0.005%
53	8.778	2389	2391	2393	rBV2	222	155	0.02%	0.002%
54	8.871	2409	2420	2447	rBV	421991	679794	70.60%	8.585%
55	9.219	2525	2528	2530	rBV	263	163	0.02%	0.002%
56	9.270	2540	2544	2547	rVB	311	215	0.02%	0.003%
57	9.302	2547	2554	2559	rVB2	313	429	0.04%	0.005%
58	9.328	2559	2562	2564	rBV2	386	263	0.03%	0.003%
59	9.482	2607	2610	2616	rVV2	381	328	0.03%	0.004%
60	9.514	2617	2620	2627	rVV2	354	418	0.04%	0.005%
61	9.563	2631	2635	2639	rVB2	254	261	0.03%	0.003%
62	9.640	2657	2659	2665	rBV2	177	187	0.02%	0.002%
63	9.974	2761	2763	2765	rBV	237	156	0.02%	0.002%
64	10.019	2774	2777	2782	rBV2	233	223	0.02%	0.003%
65	10.048	2782	2786	2789	rBV2	313	212	0.02%	0.003%
66	10.090	2796	2799	2800	rBV	275	171	0.02%	0.002%
67	10.119	2805	2808	2810	rBV2	228	166	0.02%	0.002%
68	10.183	2825	2828	2831	rBV	306	237	0.02%	0.003%
69	10.238	2833	2845	2867	rVV	266270	425034	44.14%	5.367%
70	10.428	2901	2904	2907	rVB	257	152	0.02%	0.002%
71	10.444	2907	2909	2913	rBV2	261	196	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV103020\
 Data File : VV019190.D
 Acq On : 30 Oct 2020 17:26
 Operator : SY/MD
 Sample : L4543-01DL 1000X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG455DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

72	10.479	2915	2920	2922	rBV2	243	270	0.03%	0.003%
73	10.527	2931	2935	2939	rVB	267	193	0.02%	0.002%
74	10.653	2969	2974	2978	rBV2	248	242	0.03%	0.003%
75	10.675	2979	2981	2987	rVB2	341	248	0.03%	0.003%
76	10.730	2995	2998	3001	rBV	273	256	0.03%	0.003%
77	10.775	3008	3012	3014	rBV	266	196	0.02%	0.002%
78	10.932	3055	3061	3064	rBV2	1019	1051	0.11%	0.013%
79	10.984	3074	3077	3081	rBV2	169	178	0.02%	0.002%
80	11.119	3116	3119	3121	rBV2	283	187	0.02%	0.002%
81	11.190	3139	3141	3145	rBV2	269	224	0.02%	0.003%
82	11.270	3155	3166	3194	rBV	425390	652827	67.80%	8.244%
83	11.453	3218	3223	3227	rVB3	447	413	0.04%	0.005%
84	11.646	3271	3283	3302	rBV	465183	729661	75.78%	9.214%
85	11.791	3324	3328	3331	rBV2	368	230	0.02%	0.003%
86	11.932	3369	3372	3373	rBV	206	131	0.01%	0.002%
87	12.280	3477	3480	3485	rBV2	185	150	0.02%	0.002%
88	12.569	3565	3570	3574	rBV	421	437	0.05%	0.006%
89	12.935	3680	3684	3687	rBV2	274	272	0.03%	0.003%
90	13.080	3724	3729	3734	rBV2	269	326	0.03%	0.004%
91	13.254	3780	3783	3785	rBV	253	201	0.02%	0.003%
92	13.434	3836	3839	3842	rBV2	322	282	0.03%	0.004%
93	13.550	3871	3875	3877	rBV	215	173	0.02%	0.002%
94	13.871	3973	3975	3977	rBV	279	136	0.01%	0.002%
95	13.977	4005	4008	4009	rBV	266	135	0.01%	0.002%
96	14.009	4016	4018	4022	rVB	355	220	0.02%	0.003%
97	14.045	4026	4029	4031	rBV2	308	202	0.02%	0.003%
98	14.238	4086	4089	4091	rBV	329	185	0.02%	0.002%
99	14.283	4100	4103	4104	rBV	290	181	0.02%	0.002%
100	14.701	4230	4233	4239	rBV	435	459	0.05%	0.006%


Sum of corrected areas: 7918828

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV103020\
Data File : VV019190.D
Acq On : 30 Oct 2020 17:26
Operator : SY/MD
Sample : L4543-01DL 1000X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG455DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

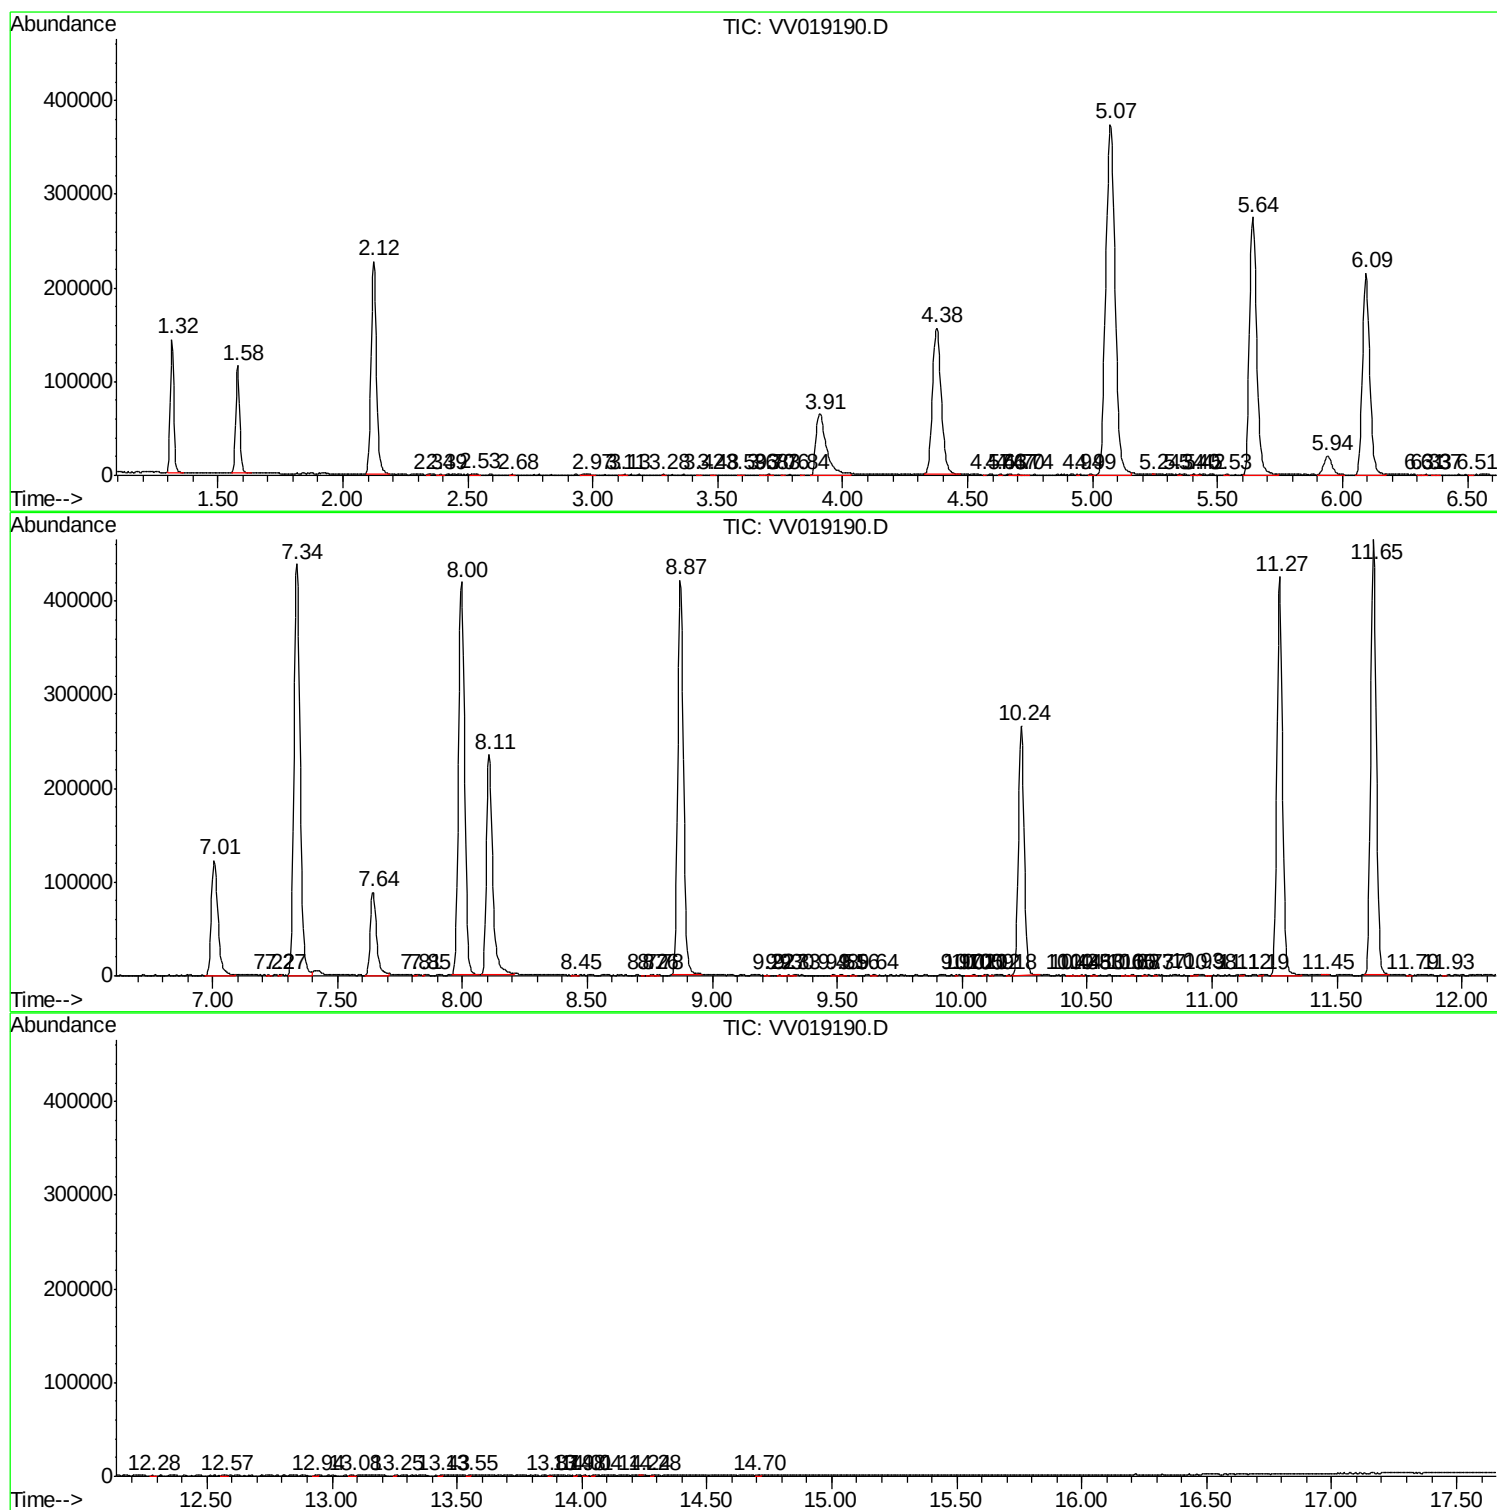

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV103020\
Data File : VV019190.D
Acq On : 30 Oct 2020 17:26
Operator : SY/MD
Sample : L4543-01DL 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG455DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV103020\
Data File : VV019190.D
Acq On : 30 Oct 2020 17:26
Operator : SY/MD
Sample : L4543-01DL 1000X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG455DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc