


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV103020\
 Data File : VV019174.D
 Acq On : 30 Oct 2020 09:18
 Operator : SY/MD
 Sample : BFB86
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB86

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis
 Last Update : Sat Oct 31 02:55:48 2020

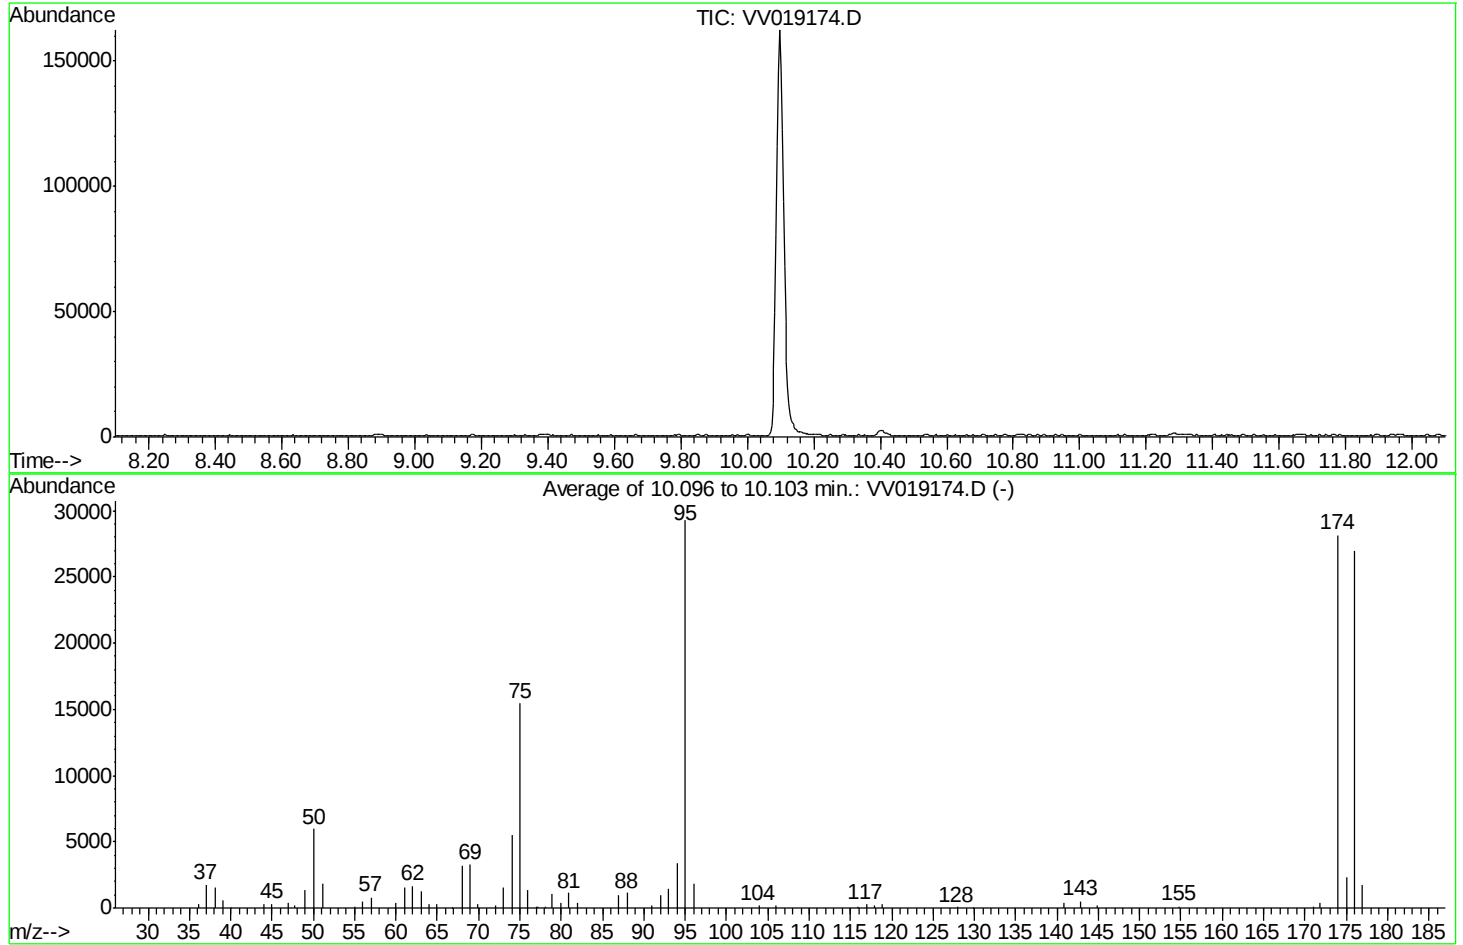

AutoFind: Scans 2801, 2802, 2803; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	5983	PASS
75	95	30	80	52.7	15419	PASS
95	95	100	100	100.0	29266	PASS
96	95	5	9	6.4	1871	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	96.2	28152	PASS
175	174	5	9	8.1	2285	PASS
176	174	95	101	95.7	26941	PASS
177	176	5	9	6.3	1698	PASS

m/z	Abundance
36.00	256.0
37.00	1869.0
38.10	1675.0
39.10	629.0
40.00	114.0
44.00	805.0
44.90	335.0
47.00	391.0
47.80	192.0
49.00	1490.0
50.10	6411.0
51.10	1923.0
55.00	152.0
56.00	514.0
57.00	821.0
60.00	414.0
61.00	1630.0
62.00	1724.0
63.00	1354.0
64.00	288.0
65.00	307.0
68.00	3263.0
69.00	3452.0
69.90	342.0
72.10	192.0
73.00	1691.0
74.00	5725.0
75.00	16148.0
76.00	1475.0
77.00	148.0
78.10	110.0
78.90	1101.0
79.90	409.0
80.90	1231.0
81.90	340.0
87.00	1010.0
88.00	1092.0
90.90	198.0
92.00	1054.0
93.00	1470.0
94.00	3447.0
95.10	30072.0
96.10	1854.0
104.00	221.0
106.00	166.0
115.80	128.0
117.00	328.0
117.90	176.0
118.90	229.0
127.90	113.0
129.80	135.0
140.90	398.0
142.90	529.0
144.90	145.0
154.90	134.0
171.00	133.0
171.90	402.0
174.00	28312.0
175.00	2279.0
176.00	27400.0
177.00	1817.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
36.10	269.0
37.00	1863.0
38.10	1656.0
39.00	593.0
40.00	133.0
44.00	798.0
44.90	331.0
47.00	395.0
47.80	201.0
49.00	1428.0
50.10	6177.0
51.10	1903.0
54.90	141.0
56.00	526.0
57.00	829.0
60.00	371.0
61.00	1615.0
62.00	1774.0
63.00	1288.0
64.00	290.0
65.00	318.0
68.00	3265.0
69.00	3348.0
69.90	327.0
72.00	187.0
73.00	1580.0
74.00	5647.0
75.00	15764.0
76.00	1363.0
76.90	133.0
77.20	153.0
78.00	142.0
78.90	1099.0
79.90	348.0
80.90	1196.0
81.90	375.0
87.00	970.0
88.00	1198.0
90.90	201.0
92.00	1043.0
93.00	1497.0
94.00	3494.0
95.10	30152.0
96.10	1930.0
103.90	197.0
106.00	192.0
115.90	108.0
116.90	295.0
118.00	175.0
118.90	263.0
127.90	114.0
140.90	403.0
142.90	557.0
144.90	142.0
154.80	134.0
171.00	105.0
171.90	406.0
174.00	29232.0
175.00	2416.0
176.00	27680.0
177.00	1727.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
36.10	283.0
37.00	1524.0
38.10	1418.0
39.00	556.0
40.10	138.0
44.00	754.0
45.00	309.0
47.00	387.0
47.80	208.0
49.00	1278.0
50.10	5362.0
51.10	1729.0
56.00	478.0
57.00	792.0
60.00	305.0
61.00	1472.0
62.00	1549.0
63.00	1150.0
64.00	244.0
64.90	266.0
66.80	100.0
68.00	2939.0
69.00	2923.0
70.00	264.0
72.00	189.0
73.00	1343.0
74.00	5023.0
75.10	14346.0
76.00	1239.0
77.20	130.0
78.00	150.0
78.90	1022.0
79.90	309.0
80.90	1040.0
81.90	341.0
87.00	947.0
87.90	1155.0
91.00	176.0
92.00	898.0
93.00	1348.0
94.00	3296.0
95.00	27576.0
96.10	1830.0
103.80	160.0
106.00	163.0
116.90	242.0
118.00	141.0
118.90	280.0
140.90	363.0
142.90	511.0
144.90	173.0
154.90	107.0
171.80	397.0
174.00	26912.0
175.00	2161.0
176.00	25744.0
177.00	1550.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

Scan 2790 (10.061 min): VV019174.D
BFB86

m/z	Abundance
40.00	115.0
44.00	463.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86