

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
 Data File : VV032761.D
 Acq On : 30 Oct 2023 10:49
 Operator : SY/MD
 Sample : 05103-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 31 02:24:52 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 31 02:23:31 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	134298	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	155618	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	67302	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	48553	4.402	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.000%
7) Chloroethane-d5	1.532	69	47087	5.024	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.400%
11) 1,1-Dichloroethene-d2	2.060	65	20361	4.113	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.200%
20) 2-Butanone-d5	3.815	46	102217	42.916	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	85.840%
24) Chloroform-d	4.256	84	90265	4.929	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.600%
26) 1,2-Dichloroethane-d4	4.947	65	46644	5.159	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.200%
32) Benzene-d6	4.963	84	179645	4.848	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.000%
36) 1,2-Dichloropropane-d6	5.992	67	53794	5.014	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.200%
41) Toluene-d8	7.246	98	163832	4.362	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.200%
43) trans-1,3-Dichloroprop...	7.561	79	21018	4.440	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.800%
46) 2-Hexanone-d5	8.030	63	79226	42.226	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.460%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	45575	4.777	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.600%
66) 1,2-Dichlorobenzene-d4	11.564	152	59316	5.397	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.000%
Target Compounds						Qvalue
61) 1,2,3-Trichloropropane	11.188	75	8492	1.193	ug/L	# 61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032761.D
Acq On : 30 Oct 2023 10:49
Operator : SY/MD
Sample : 05103-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 31 02:24:52 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 31 02:23:31 2023
Response via : Initial Calibration

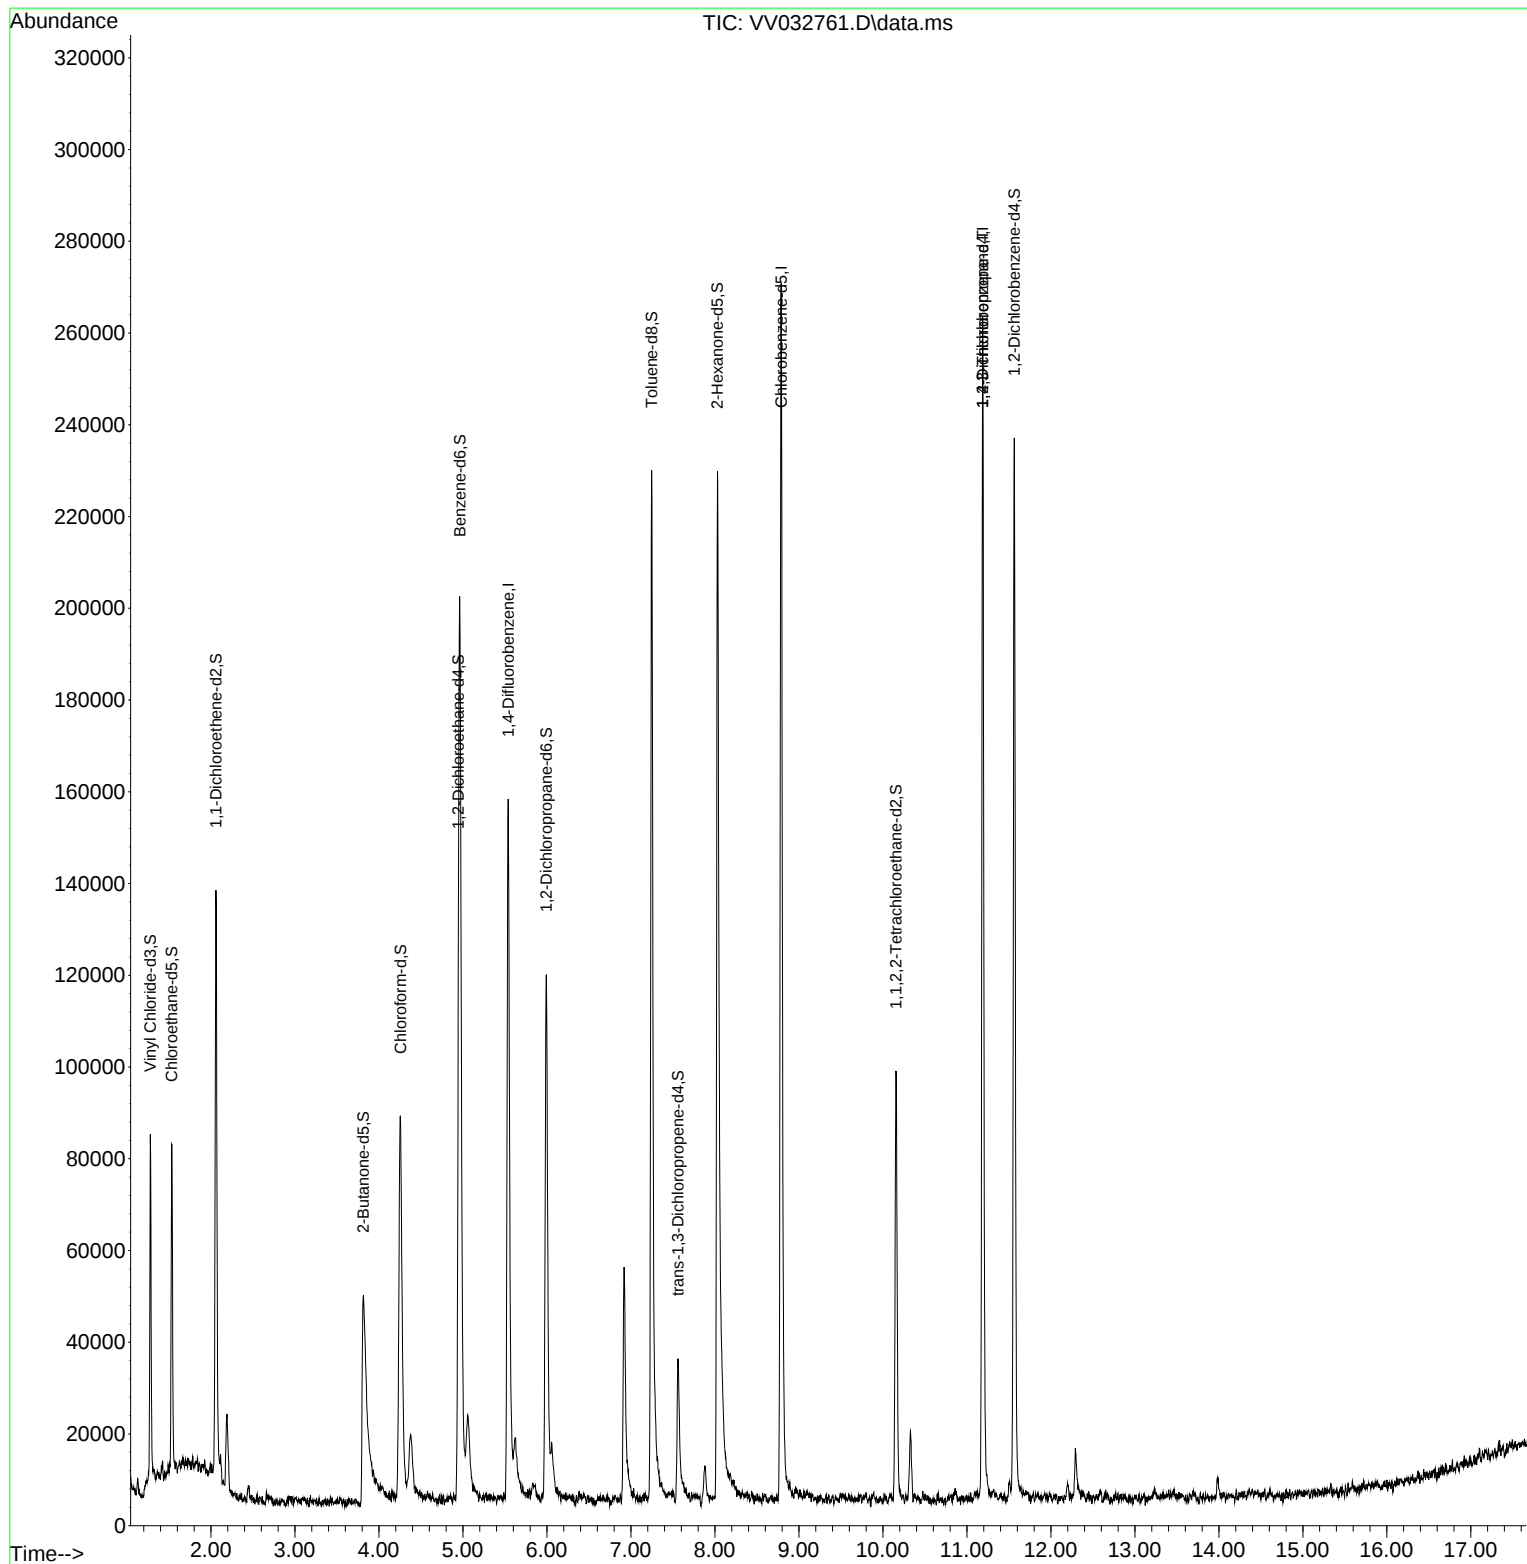

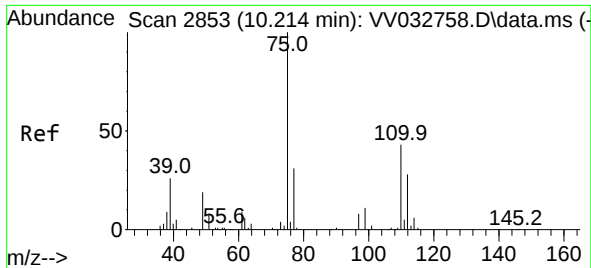

#61

1,2,3-Trichloropropane

Concen: 1.193 ug/L

RT: 11.188 min Scan# 31

Delta R.T. 0.974 min


Lab File: VV032761.D

Acq: 30 Oct 2023 10:49

Instrument :

MSVOA_V

ClientSampleId :

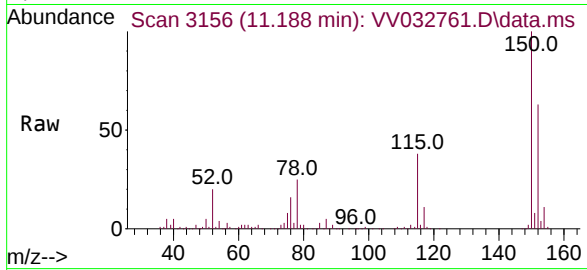

Tgt Ion: 75 Resp: 8492

Ion Ratio Lower Upper

75 100

77 37.5 24.5 36.7#

110 3.5 32.3 48.5#

