

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
 Data File : VV032766.D
 Acq On : 30 Oct 2023 12:51
 Operator : SY/MD
 Sample : 05103-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 31 02:25:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 31 02:23:31 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	125452	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	149050	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	64248	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	44742	4.343	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	86.800%	
7) Chloroethane-d5	1.532	69	44317	5.061	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	101.200%	
11) 1,1-Dichloroethene-d2	2.060	65	19012	4.111	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	82.200%	
20) 2-Butanone-d5	3.809	46	92545	41.595	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	83.180%	
24) Chloroform-d	4.252	84	86828	5.075	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.600%	
26) 1,2-Dichloroethane-d4	4.950	65	42003	4.973	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	99.400%	
32) Benzene-d6	4.963	84	170257	4.798	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.000%	
36) 1,2-Dichloropropane-d6	5.992	67	51915	5.052	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	101.000%	
41) Toluene-d8	7.246	98	153015	4.254	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.000%	
43) trans-1,3-Dichloroprop...	7.561	79	20081	4.429	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	88.600%	
46) 2-Hexanone-d5	8.030	63	72471	40.328	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	80.660%	
56) 1,1,2,2-Tetrachloroeth...	10.159	84	42503	4.651	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	93.000%	
66) 1,2-Dichlorobenzene-d4	11.564	152	56881	5.422	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	108.400%	
Target Compounds						
61) 1,2,3-Trichloropropane	11.191	75	7682	1.131	ug/L	Qvalue # 56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032766.D
Acq On : 30 Oct 2023 12:51
Operator : SY/MD
Sample : 05103-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 31 02:25:55 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 31 02:23:31 2023
Response via : Initial Calibration

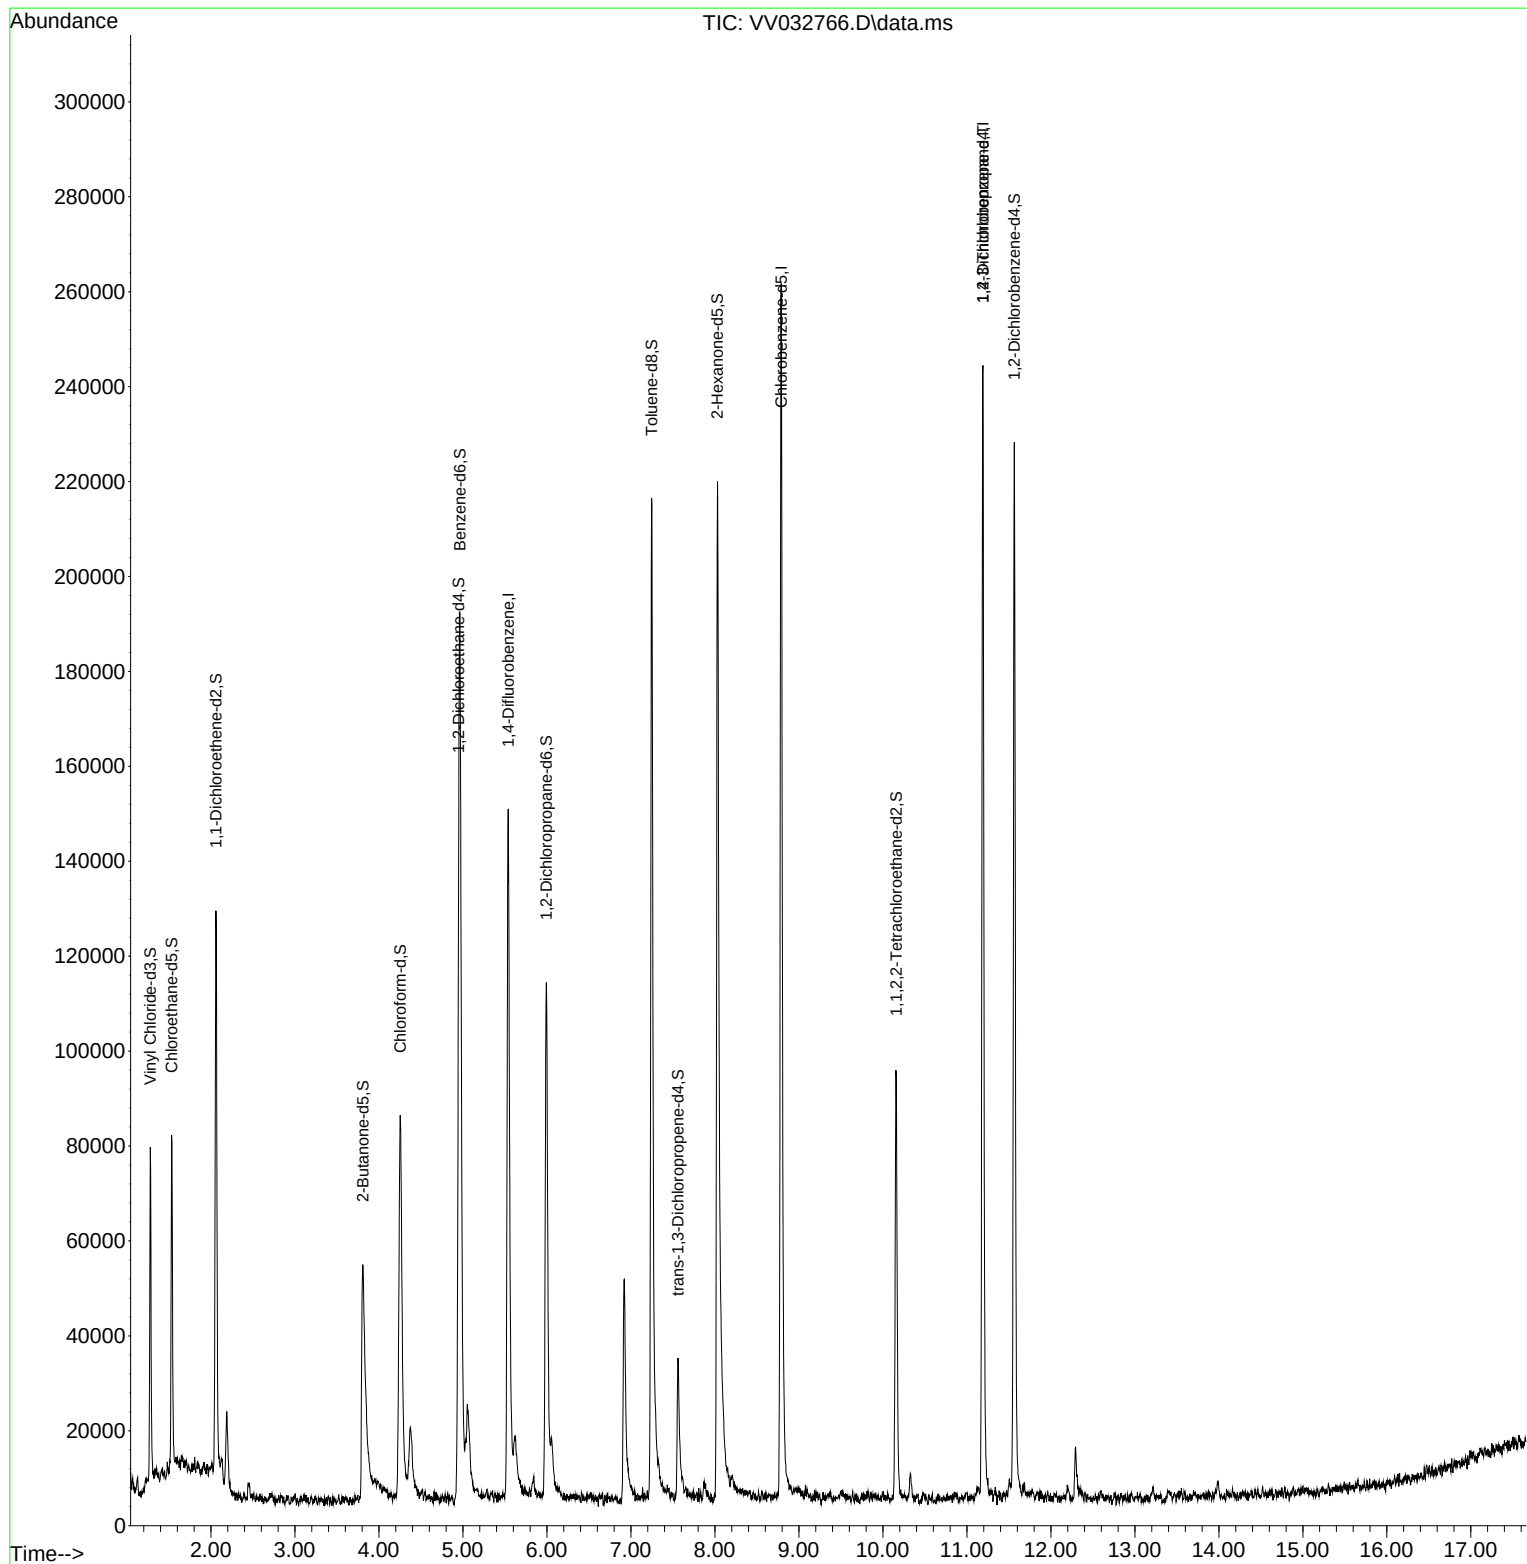

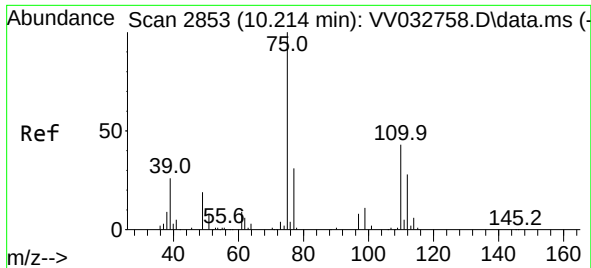

#61
 1,2,3-Trichloropropane
 Concen: 1.131 ug/L
 RT: 11.191 min Scan# 31
 Delta R.T. 0.977 min
 Lab File: VV032766.D
 Acq: 30 Oct 2023 12:51

Instrument :
 MSVOA_V
 ClientSampleId :

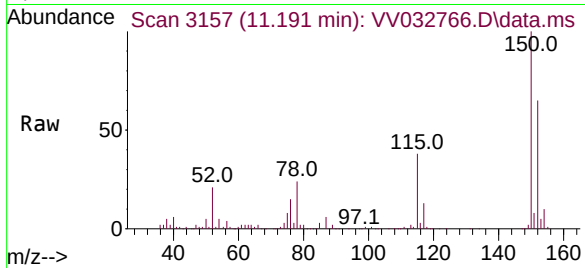

Tgt Ion: 75 Resp: 7682
 Ion Ratio Lower Upper
 75 100
 77 42.7 24.5 36.7#
 110 2.6 32.3 48.5#

