




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
 Data File : VV032773.D
 Acq On : 30 Oct 2023 15:42
 Operator : SY/MD
 Sample : 05114-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B60

Manual IntegrationsAPPROVED

Quant Time: Oct 31 02:27:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 31 02:23:31 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/31/2023
 Supervised By :Mahesh Dadoda 11/01/2023

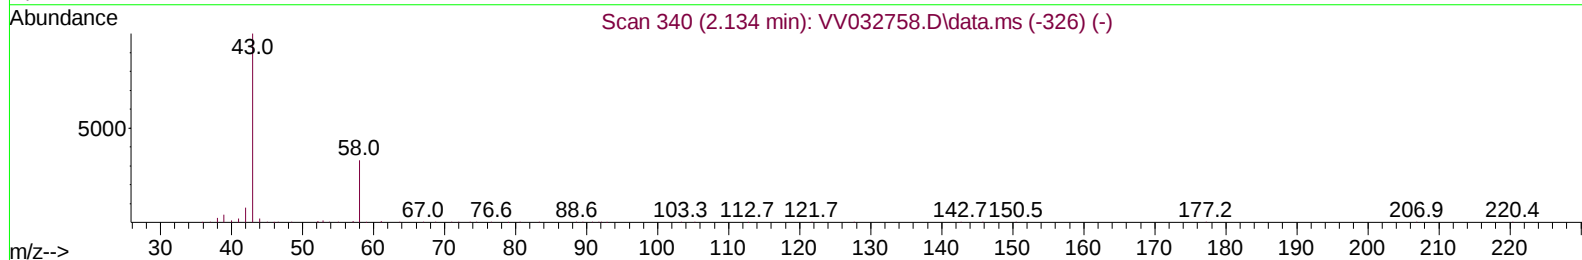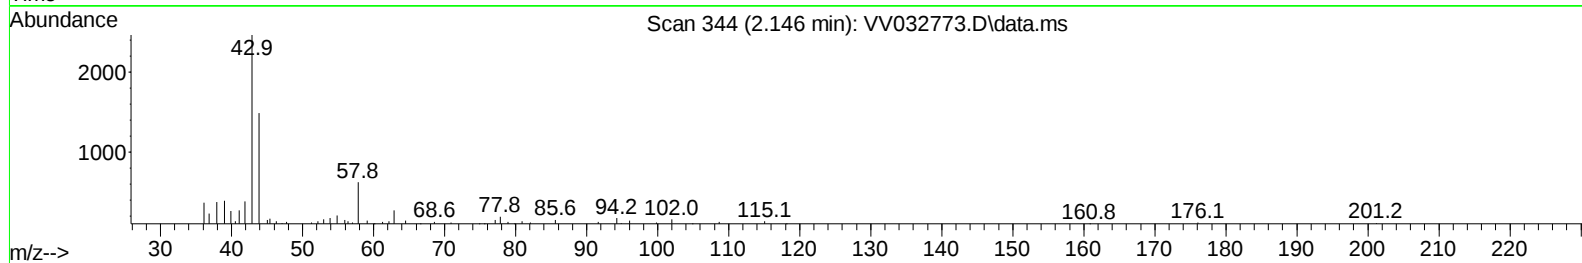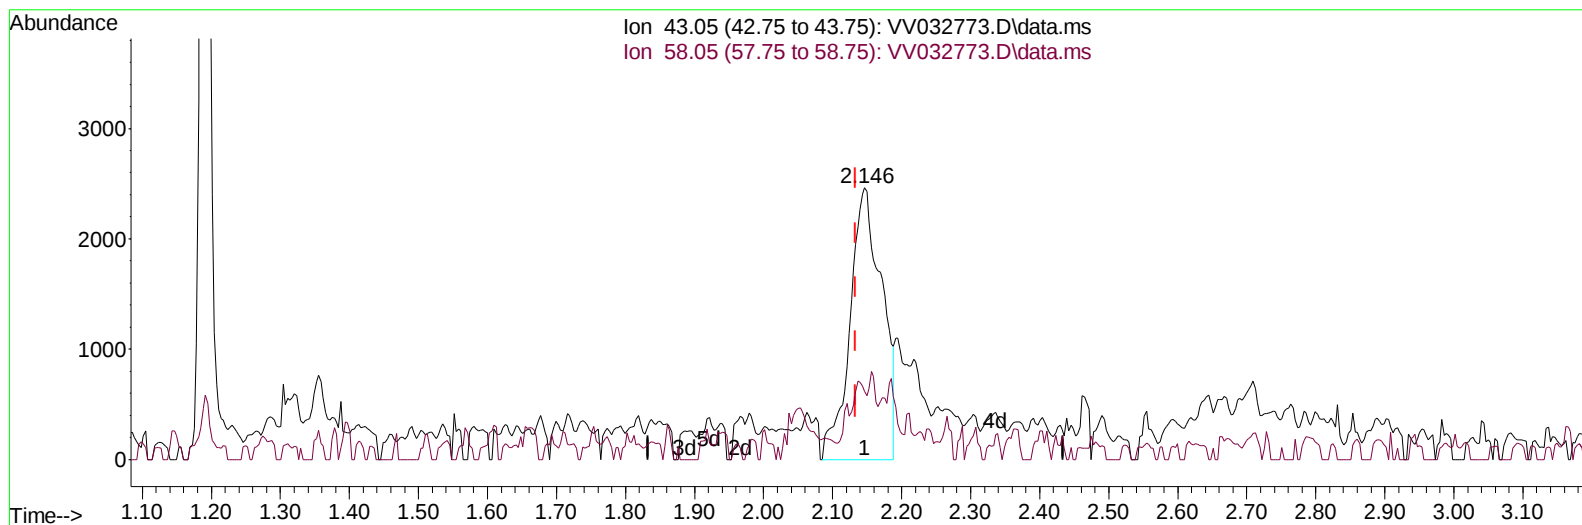

TIC: VV032773.D\data.ms

(13) Acetone (T)

2.146min (+ 0.013) 3.80 ug/L

response 7946

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	25.30	6.22
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
 Data File : VV032773.D
 Acq On : 30 Oct 2023 15:42
 Operator : SY/MD
 Sample : 05114-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B60

Manual IntegrationsAPPROVED

Quant Time: Oct 31 02:27:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 31 02:23:31 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/31/2023
 Supervised By :Mahesh Dadoda 11/01/2023

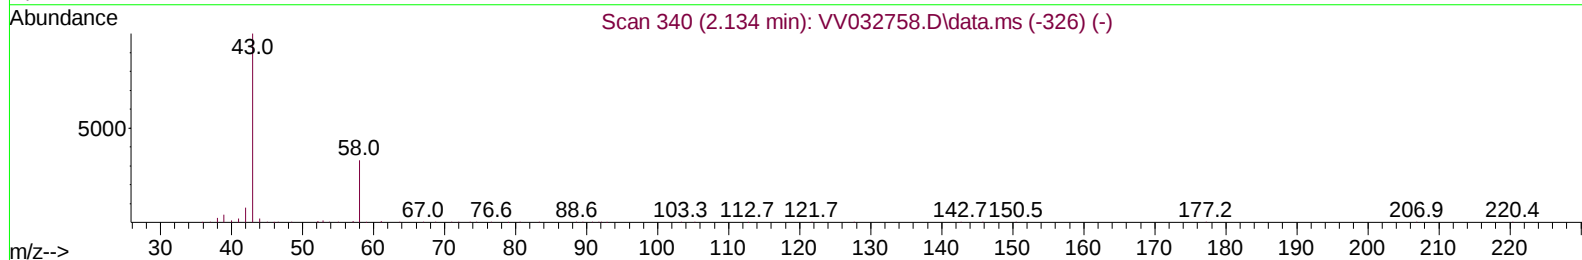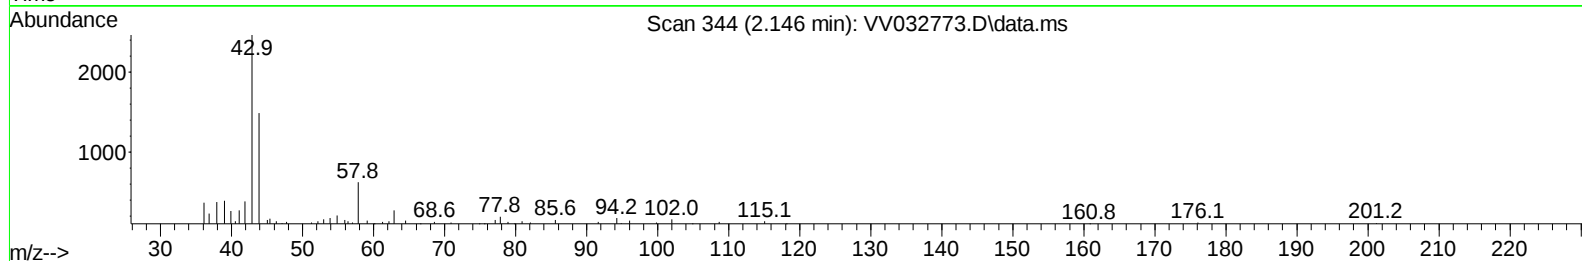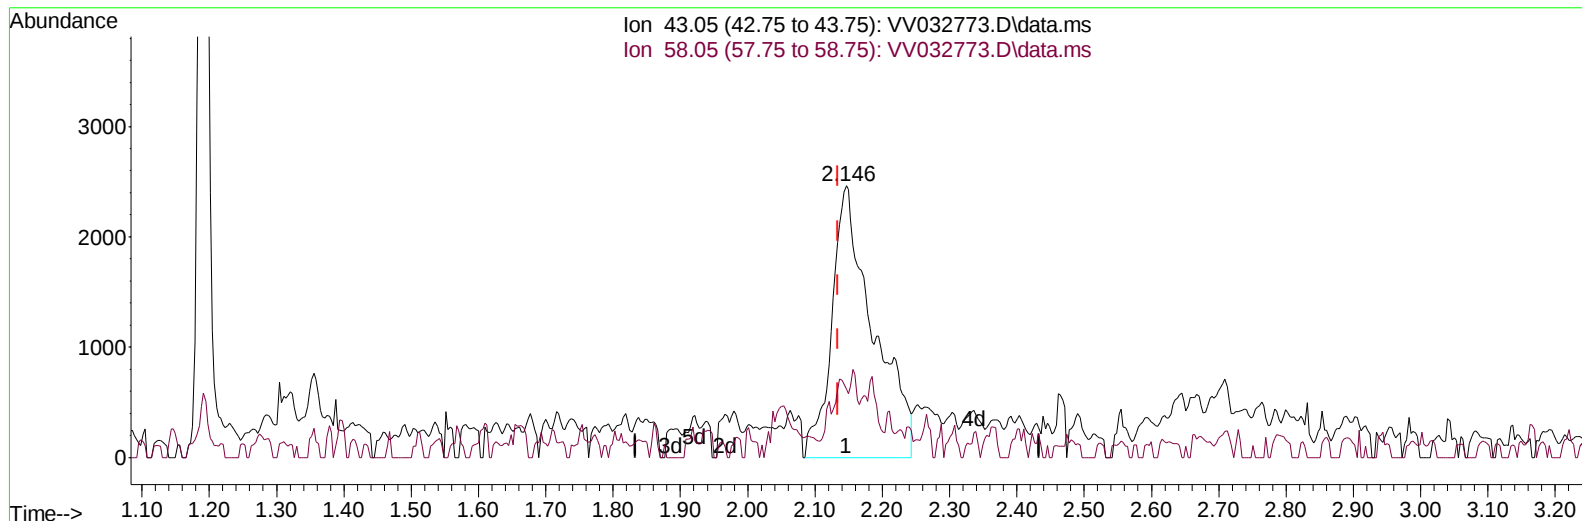

TIC: VV032773.D\data.ms

(13) Acetone (T)

2.146min (+ 0.013) 5.01 ug/L m

response 10480

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	25.30	4.71
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
 Data File : VV032773.D
 Acq On : 30 Oct 2023 15:42
 Operator : SY/MD
 Sample : 05114-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B60

Manual IntegrationsAPPROVED

Quant Time: Oct 31 02:27:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 31 02:23:31 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/31/2023
 Supervised By :Mahesh Dadoda 11/01/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	119465	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	140052	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	60631	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	43696	4.454	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	89.000%		
7) Chloroethane-d5	1.532	69	42885	5.143	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	102.800%		
11) 1,1-Dichloroethene-d2	2.060	65	19876	4.513	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	90.200%		
20) 2-Butanone-d5	3.822	46	90394	42.664	ug/L	0.02
Spiked Amount 50.000	Range 40 - 130		Recovery =	85.320%		
24) Chloroform-d	4.252	84	101241	6.214	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	124.200%		
26) 1,2-Dichloroethane-d4	4.947	65	43422	5.399	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	108.000%		
32) Benzene-d6	4.963	84	164190	4.924	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	98.400%		
36) 1,2-Dichloropropane-d6	5.992	67	50824	5.264	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	105.200%		
41) Toluene-d8	7.246	98	147256	4.357	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	87.200%		
43) trans-1,3-Dichloroprop...	7.561	79	19120	4.488	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	89.800%		
46) 2-Hexanone-d5	8.030	63	75270	44.577	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	89.160%		
56) 1,1,2,2-Tetrachloroeth...	10.156	84	43904	5.113	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	102.200%		
66) 1,2-Dichlorobenzene-d4	11.564	152	55403	5.596	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	112.000%		
Target Compounds						
						Qvalue
13) Acetone	2.146	43	10480m	5.010	ug/L	
25) Chloroform	4.278	83	290814	14.290	ug/L	99
38) Bromodichloromethane	6.436	83	50455	3.206	ug/L	99
49) Dibromochloromethane	8.182	129	9172	0.859	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032773.D
Acq On : 30 Oct 2023 15:42
Operator : SY/MD
Sample : 05114-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B60

Manual IntegrationsAPPROVED

Quant Time: Oct 31 02:27:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 31 02:23:31 2023
Response via : Initial Calibration

Reviewed By :John Carlone 10/31/2023
Supervised By :Mahesh Dadoda 11/01/2023

