

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
 Data File : VV032762.D
 Acq On : 30 Oct 2023 11:13
 Operator : SY/MD
 Sample : 05103-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49Y5

Quant Time: Oct 31 02:25:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 31 02:23:31 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	130634	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	153237	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	67610	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	50054	4.666	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.400%
7) Chloroethane-d5	1.535	69	49482	5.427	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.600%
11) 1,1-Dichloroethene-d2	2.063	65	19950	4.143	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.800%
20) 2-Butanone-d5	3.799	46	95539	41.237	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	82.480%
24) Chloroform-d	4.256	84	91168	5.118	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.400%
26) 1,2-Dichloroethane-d4	4.947	65	47087	5.354	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.000%
32) Benzene-d6	4.963	84	181002	4.961	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.200%
36) 1,2-Dichloropropane-d6	5.992	67	56004	5.301	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.000%
41) Toluene-d8	7.246	98	166592	4.505	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.000%
43) trans-1,3-Dichloroprop...	7.561	79	19992	4.288	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.800%
46) 2-Hexanone-d5	8.027	63	77570	41.986	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.980%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	44813	4.770	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.400%
66) 1,2-Dichlorobenzene-d4	11.564	152	62868	5.695	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	113.800%
Target Compounds						Qvalue
13) Acetone	2.124	43	5202	2.274	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032762.D
Acq On : 30 Oct 2023 11:13
Operator : SY/MD
Sample : 05103-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49Y5

Quant Time: Oct 31 02:25:04 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 31 02:23:31 2023
Response via : Initial Calibration

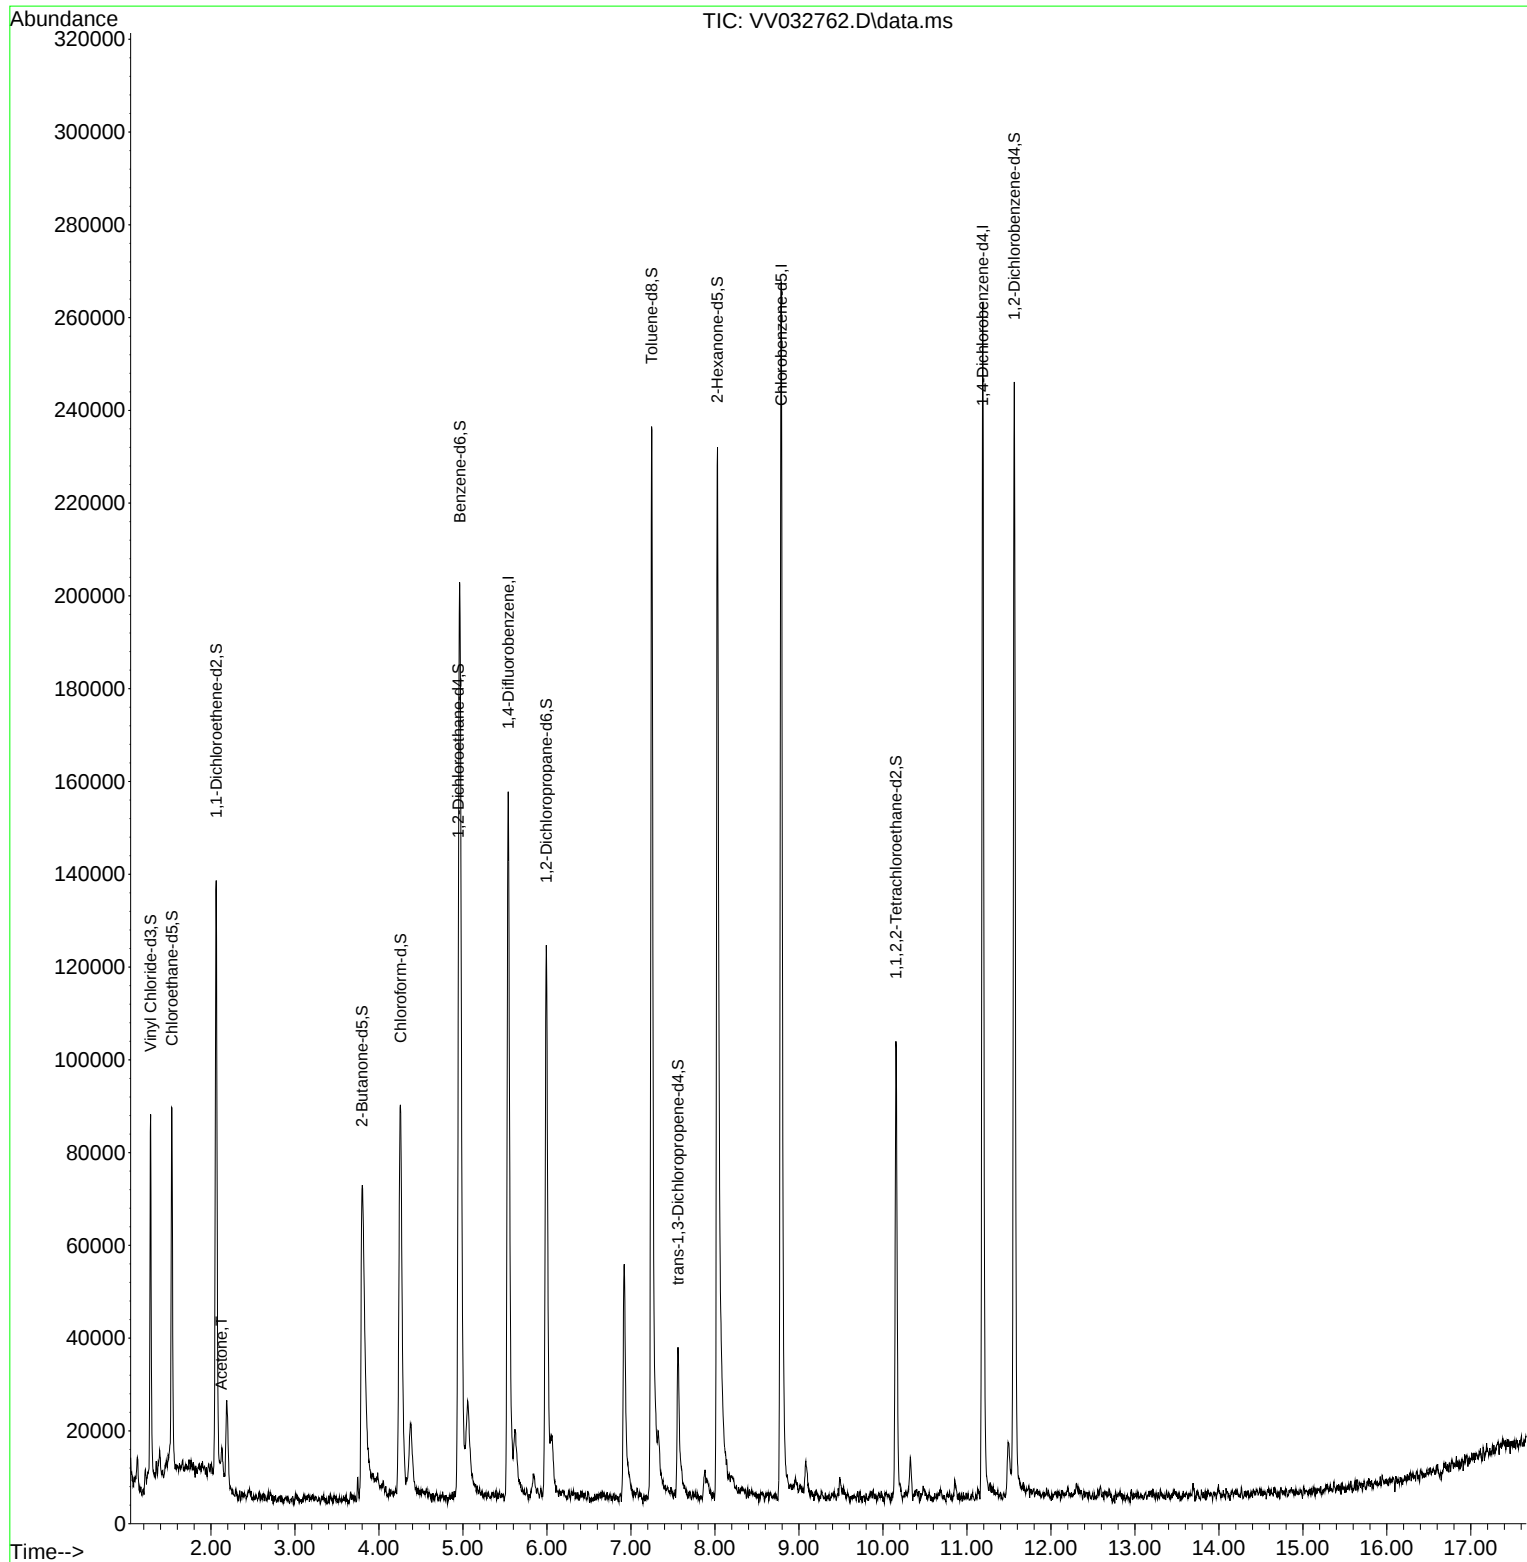

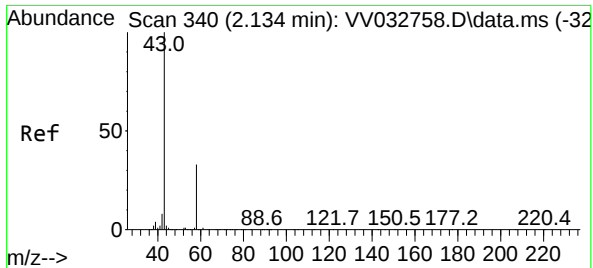

#13
Acetone
Concen: 2.274 ug/L
RT: 2.124 min Scan# 31
Delta R.T. -0.010 min
Lab File: VV032762.D
Acq: 30 Oct 2023 11:13

Instrument :
MSVOA_V
ClientSampleId :
A49Y5

Tgt Ion: 43 Resp: 5202
Ion Ratio Lower Upper
43 100
58 29.7 0.0 50.6

