

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
 Data File : VV032760.D
 Acq On : 30 Oct 2023 10:24
 Operator : SY/MD
 Sample : 05103-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49J5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032760.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	49	55	64	rBV	14760	19151	3.42%	0.386%
2	1.278	67	74	86	rVV	72961	79210	14.16%	1.595%
3	1.532	146	153	162	rVB	70318	81048	14.49%	1.632%
4	2.059	308	317	330	rBV	121888	179386	32.07%	3.611%
5	2.124	335	337	345	rVV5	6694	7779	1.39%	0.157%
6	2.182	348	355	367	rVB2	19368	37505	6.70%	0.755%
7	3.812	842	862	895	rBV3	114942	433659	77.52%	8.730%
8	4.252	984	999	1021	rBV2	80761	212880	38.05%	4.286%
9	4.371	1025	1036	1049	rVB2	11424	29845	5.33%	0.601%
10	4.960	1203	1219	1237	rBV2	188564	480595	85.91%	9.675%
11	5.053	1240	1248	1264	rVB4	15353	42103	7.53%	0.848%
12	5.535	1385	1398	1416	rBV	179578	383848	68.62%	7.727%
13	5.992	1525	1540	1554	rBV2	114243	238960	42.72%	4.811%
14	6.918	1818	1828	1841	rBV2	50505	99134	17.72%	1.996%
15	7.246	1919	1930	1953	rBV	217199	419837	75.05%	8.452%
16	7.561	2019	2028	2040	rBV	31331	58899	10.53%	1.186%
17	7.873	2119	2125	2136	rBV3	6770	11691	2.09%	0.235%
18	8.030	2164	2174	2212	rBV	202003	469348	83.90%	9.449%
19	8.786	2397	2409	2429	rBV	319666	559422	100.00%	11.262%
20	10.156	2825	2835	2855	rVB	88852	150951	26.98%	3.039%
21	10.329	2877	2889	2900	rBV3	17676	30869	5.52%	0.621%
22	11.188	3144	3156	3177	rBV	312310	502408	89.81%	10.114%
23	11.291	3182	3188	3196	rVB	5478	8599	1.54%	0.173%
24	11.493	3244	3251	3257	rBV10	6750	9724	1.74%	0.196%
25	11.564	3262	3273	3290	rVB	231360	368802	65.93%	7.425%
26	11.953	3383	3394	3404	rBV	6405	13164	2.35%	0.265%
27	12.201	3460	3471	3479	rBV	7837	12998	2.32%	0.262%
28	14.355	4129	4141	4151	rBV9	13875	25529	4.56%	0.514%




Sum of corrected areas: 4967344

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032760.D
Acq On : 30 Oct 2023 10:24
Operator : SY/MD
Sample : 05103-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49J5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

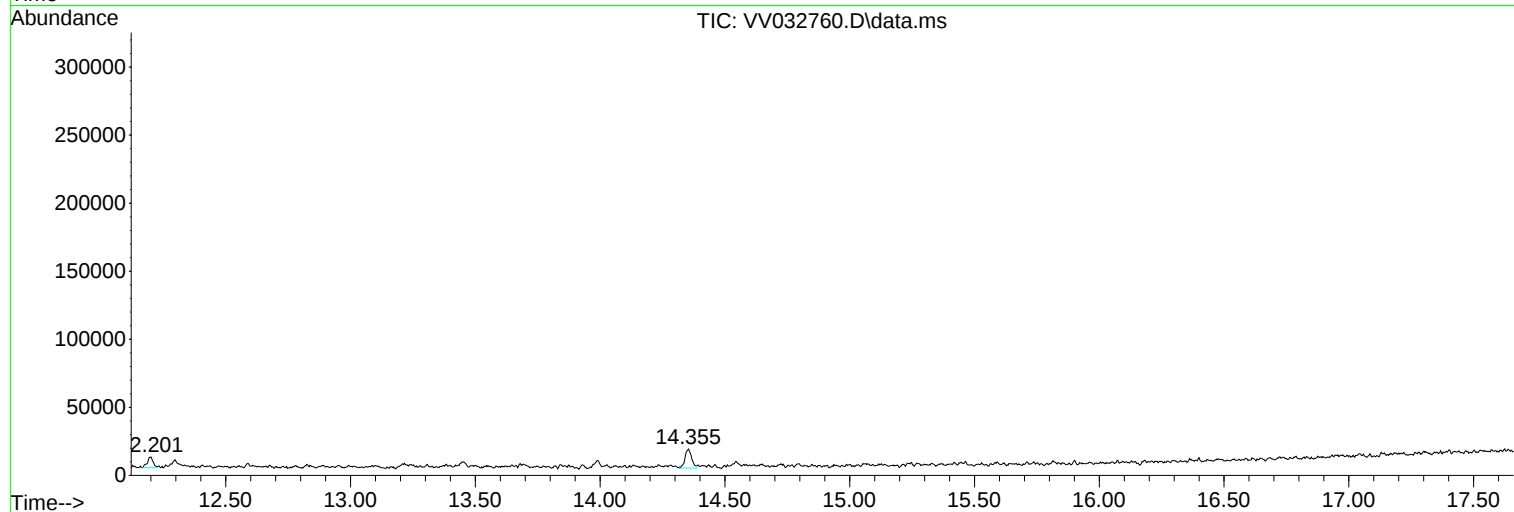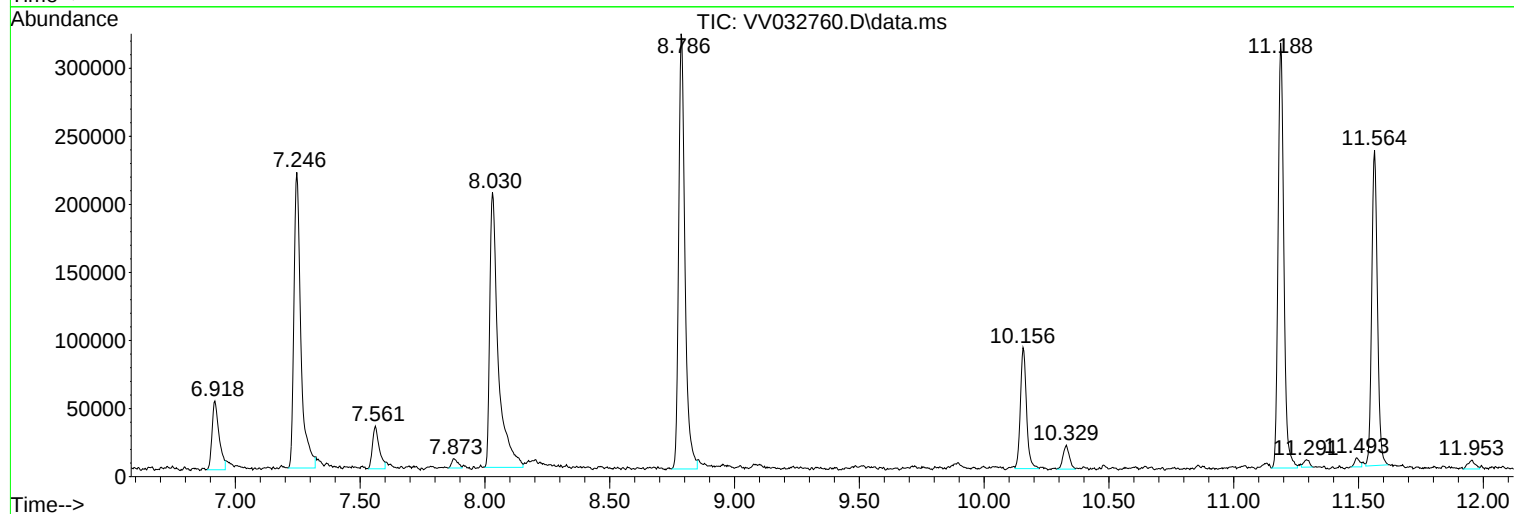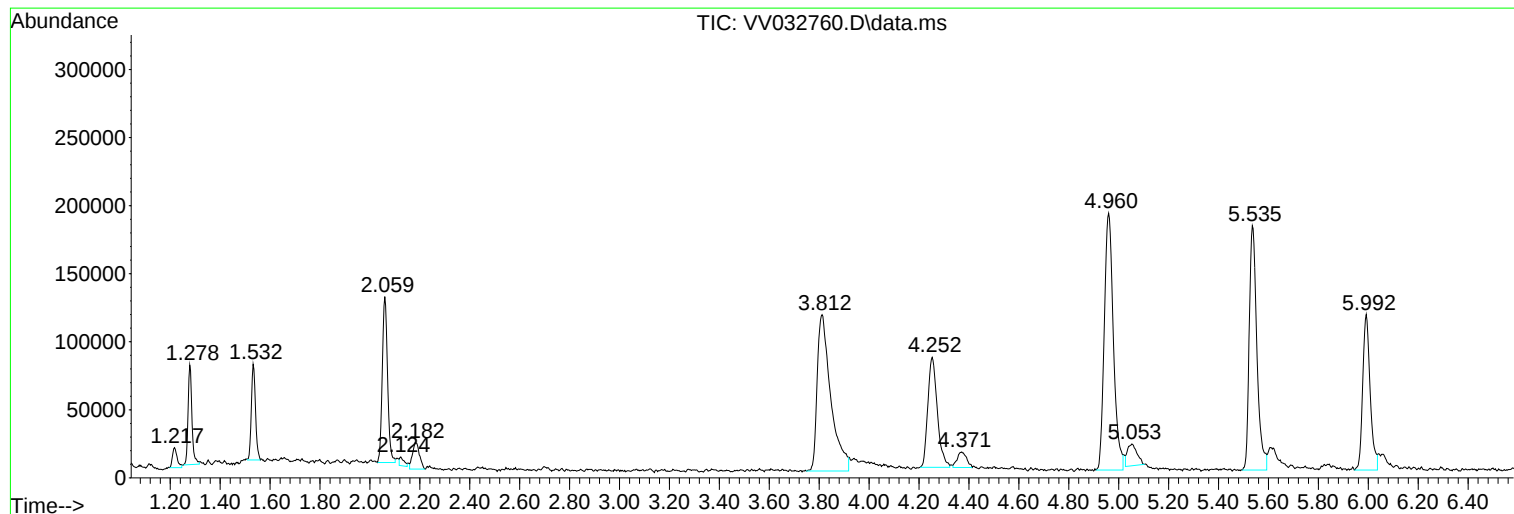

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032760.D
Acq On : 30 Oct 2023 10:24
Operator : SY/MD
Sample : 05103-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49J5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032760.D
Acq On : 30 Oct 2023 10:24
Operator : SY/MD
Sample : 05103-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49J5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc