

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
 Data File : VV032763.D
 Acq On : 30 Oct 2023 11:38
 Operator : SY/MD
 Sample : 05103-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49Y7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032763.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	21	27	33	rVB	6244	8658	1.84%	0.198%
2	1.217	49	55	64	rBV2	18684	25981	5.51%	0.593%
3	1.281	67	75	87	rVV	71424	81725	17.33%	1.864%
4	1.384	104	107	116	rVB2	8347	8713	1.85%	0.199%
5	1.535	147	154	168	rVB	74378	87502	18.55%	1.996%
6	2.063	308	318	329	rBV	117458	169649	35.97%	3.870%
7	2.188	347	357	365	rVB2	16259	26488	5.62%	0.604%
8	3.805	848	860	883	rBV3	64249	210974	44.73%	4.813%
9	4.256	984	1000	1020	rBV2	79235	205475	43.56%	4.688%
10	4.371	1027	1036	1037	rBV7	10747	12662	2.68%	0.289%
11	4.963	1204	1220	1237	rBV2	183365	464352	98.44%	10.594%
12	5.056	1240	1249	1265	rVB6	15887	44717	9.48%	1.020%
13	5.539	1386	1399	1416	rBV	150410	321683	68.20%	7.339%
14	5.622	1418	1425	1434	rVB4	9132	20548	4.36%	0.469%
15	5.834	1483	1491	1502	rBV4	5985	11073	2.35%	0.253%
16	5.995	1527	1541	1554	rBV	110114	232871	49.37%	5.313%
17	6.921	1816	1829	1845	rBV	49563	105866	22.44%	2.415%
18	7.249	1919	1931	1952	rBV	206603	409681	86.85%	9.346%
19	7.561	2016	2028	2042	rBV3	30781	64257	13.62%	1.466%
20	7.879	2119	2127	2130	rBV8	3755	5233	1.11%	0.119%
21	8.030	2165	2174	2207	rBV	203433	471703	100.00%	10.761%
22	8.789	2398	2410	2427	rBV	262636	459817	97.48%	10.490%
23	9.085	2495	2502	2511	rVB	4439	6051	1.28%	0.138%
24	10.156	2826	2835	2848	rBV	89972	147134	31.19%	3.357%
25	10.326	2880	2888	2898	rBV4	6314	10921	2.32%	0.249%
26	11.188	3145	3156	3173	rBV	253420	408745	86.65%	9.325%
27	11.564	3263	3273	3292	rVB	226159	360857	76.50%	8.232%




Sum of corrected areas: 4383336

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032763.D
Acq On : 30 Oct 2023 11:38
Operator : SY/MD
Sample : 05103-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49Y7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

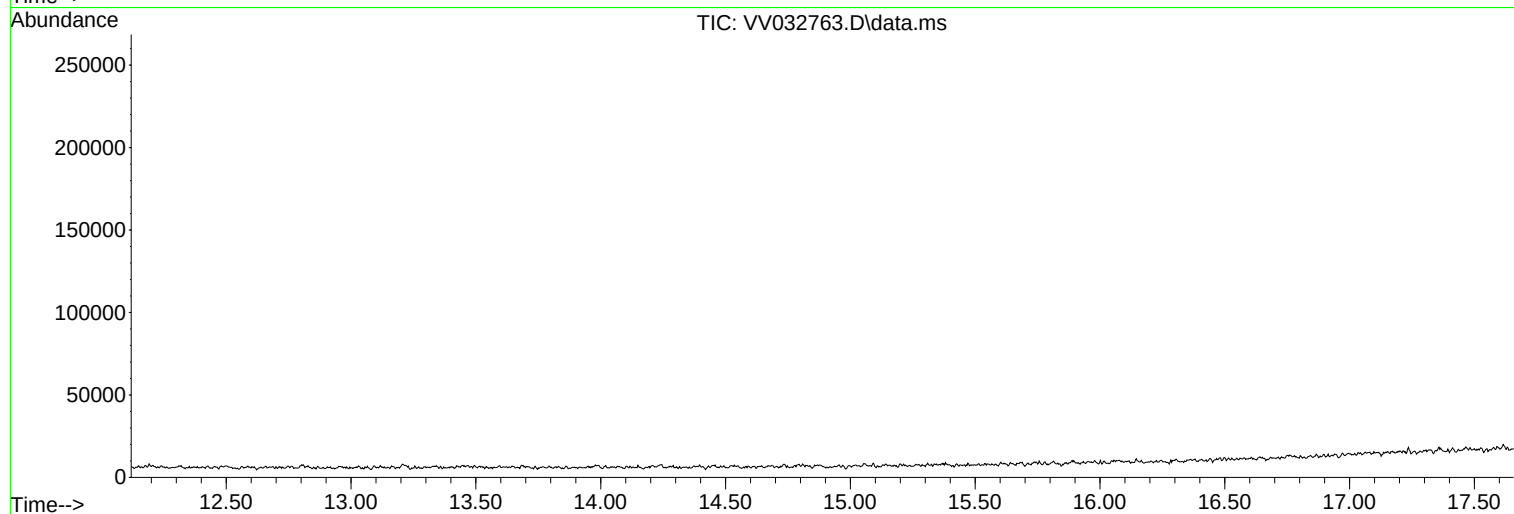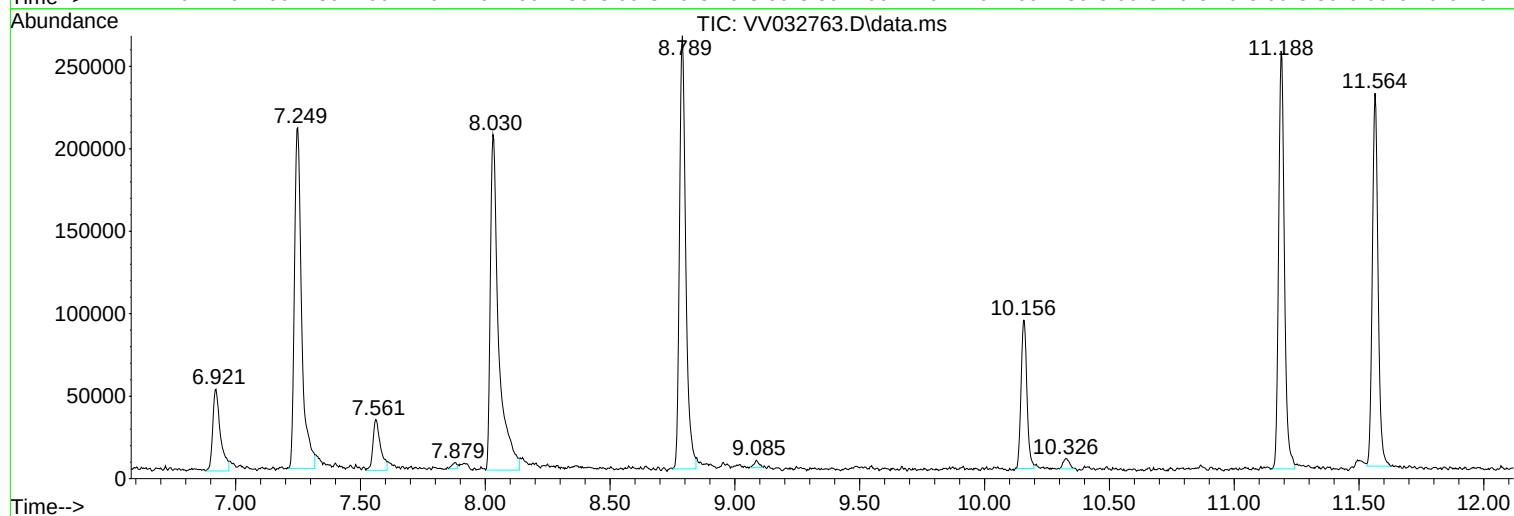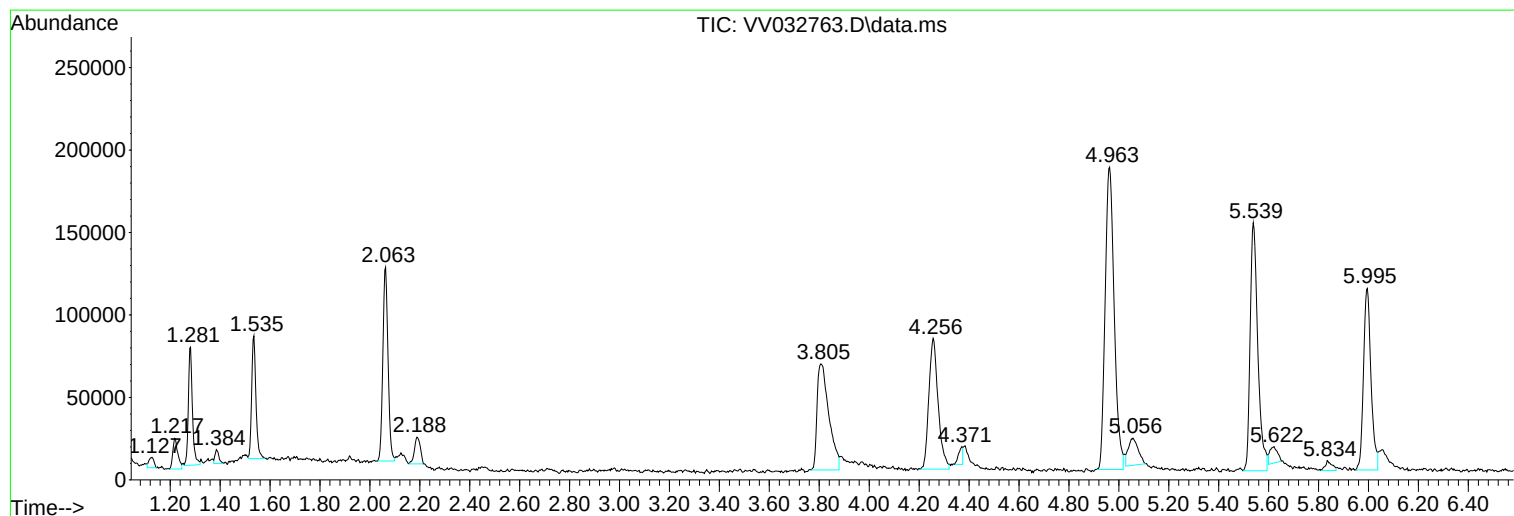

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032763.D
Acq On : 30 Oct 2023 11:38
Operator : SY/MD
Sample : 05103-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49Y7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032763.D
Acq On : 30 Oct 2023 11:38
Operator : SY/MD
Sample : 05103-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49Y7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc