

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
 Data File : VV032766.D
 Acq On : 30 Oct 2023 12:51
 Operator : SY/MD
 Sample : 05103-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4A56

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032766.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	83	rBV	69766	74991	15.37%	1.787%
2	1.532	143	153	164	rBV	71346	86859	17.80%	2.070%
3	2.060	308	317	327	rBV	116985	166879	34.20%	3.978%
4	2.188	347	357	367	rVB2	15666	26645	5.46%	0.635%
5	3.809	851	861	892	rBV	49053	161004	32.99%	3.838%
6	4.256	985	1000	1021	rBV	80295	214406	43.94%	5.110%
7	4.375	1027	1037	1052	rVB3	11504	27656	5.67%	0.659%
8	4.963	1203	1220	1238	rBV2	186424	471008	96.52%	11.227%
9	5.539	1386	1399	1417	rBV	145291	309093	63.34%	7.367%
10	5.992	1529	1540	1555	rBV2	107857	229752	47.08%	5.476%
11	6.921	1817	1829	1840	rBV	47277	95193	19.51%	2.269%
12	7.246	1918	1930	1953	rBV	211024	411744	84.38%	9.814%
13	7.561	2019	2028	2042	rBV	29446	58070	11.90%	1.384%
14	8.030	2165	2174	2206	rBV2	214026	487966	100.00%	11.631%
15	8.789	2398	2410	2434	rBV	255500	449815	92.18%	10.722%
16	10.156	2824	2835	2851	rBV	90470	152705	31.29%	3.640%
17	10.326	2882	2888	2897	rVB8	5094	7588	1.56%	0.181%
18	11.191	3146	3157	3174	rBV	237602	390607	80.05%	9.310%
19	11.564	3261	3273	3293	rVV	220773	357803	73.33%	8.528%
20	12.294	3489	3500	3504	rBV	11165	15622	3.20%	0.372%




Sum of corrected areas: 4195406

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032766.D
Acq On : 30 Oct 2023 12:51
Operator : SY/MD
Sample : 05103-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4A56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

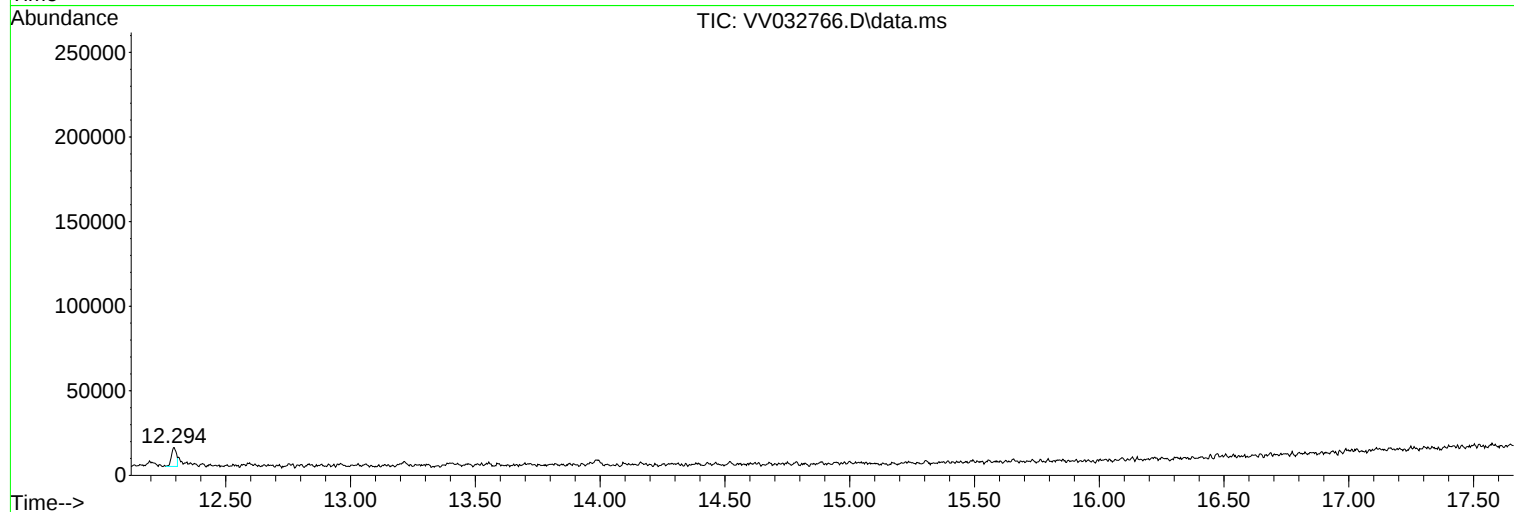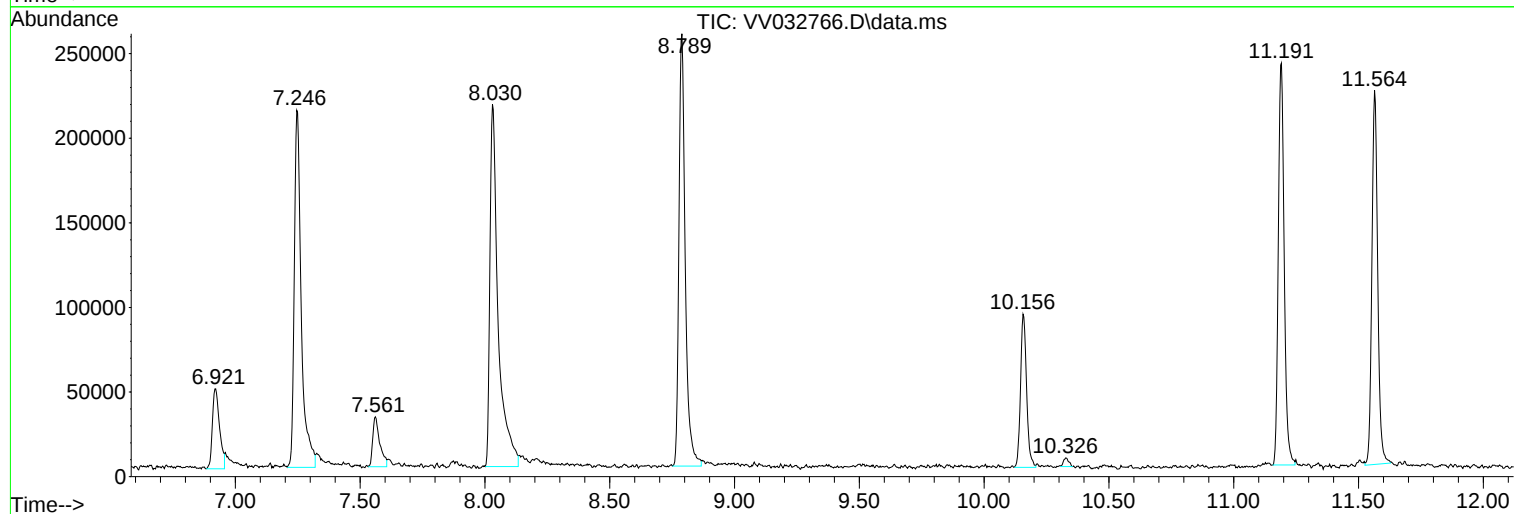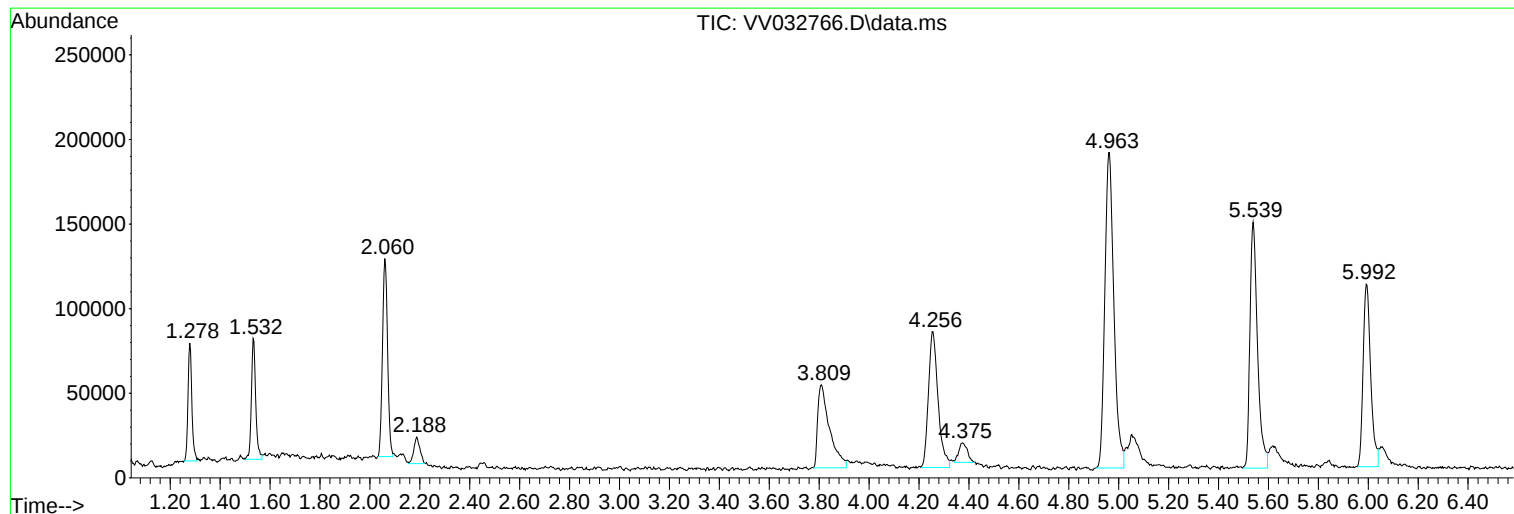

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032766.D
Acq On : 30 Oct 2023 12:51
Operator : SY/MD
Sample : 05103-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4A56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032766.D
Acq On : 30 Oct 2023 12:51
Operator : SY/MD
Sample : 05103-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4A56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc