

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
 Data File : VV032769.D
 Acq On : 30 Oct 2023 14:04
 Operator : SY/MD
 Sample : 05019-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032769.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.133	20	29	35	rBV	8607	11849	2.43%	0.294%
2	1.278	67	74	83	rVV	61989	65677	13.48%	1.630%
3	1.506	138	145	148	rBV	16963	19505	4.00%	0.484%
4	1.532	148	153	167	rVB	72453	87008	17.86%	2.159%
5	2.059	308	317	327	rBV	99739	143224	29.40%	3.555%
6	2.198	351	360	374	rBV	12906	23906	4.91%	0.593%
7	2.445	431	437	445	rBV6	6175	9866	2.03%	0.245%
8	3.825	850	866	889	rBV2	13137	49191	10.10%	1.221%
9	4.252	984	999	1021	rBV	77912	208135	42.73%	5.166%
10	4.387	1028	1041	1051	rBV2	12652	32448	6.66%	0.805%
11	4.960	1203	1219	1239	rBV3	168381	444995	91.36%	11.044%
12	5.063	1242	1251	1267	rVB6	15823	43363	8.90%	1.076%
13	5.538	1386	1399	1418	rBV2	161696	343812	70.59%	8.533%
14	5.619	1418	1424	1439	rVB2	10420	25844	5.31%	0.641%
15	5.825	1480	1488	1489	rBV8	5523	5207	1.07%	0.129%
16	5.992	1529	1540	1556	rVV2	111510	237824	48.83%	5.902%
17	6.053	1557	1559	1574	rVB9	10794	22174	4.55%	0.550%
18	6.921	1819	1829	1846	rBV2	34703	75040	15.41%	1.862%
19	7.246	1920	1930	1953	rBV	176531	335222	68.82%	8.320%
20	7.564	2021	2029	2038	rBV	21942	38264	7.86%	0.950%
21	8.034	2159	2175	2207	rBV2	165247	397821	81.68%	9.873%
22	8.368	2269	2279	2285	rBV7	10408	16529	3.39%	0.410%
23	8.789	2398	2410	2428	rBV	271639	487074	100.00%	12.088%
24	10.159	2825	2836	2850	rBV	102048	171746	35.26%	4.262%
25	10.329	2882	2889	2897	rVB8	4786	7710	1.58%	0.191%
26	11.188	3145	3156	3178	rBV	249819	403161	82.77%	10.006%
27	11.564	3262	3273	3293	rBV	197727	322663	66.25%	8.008%




Sum of corrected areas: 4029258

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032769.D
Acq On : 30 Oct 2023 14:04
Operator : SY/MD
Sample : 05019-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

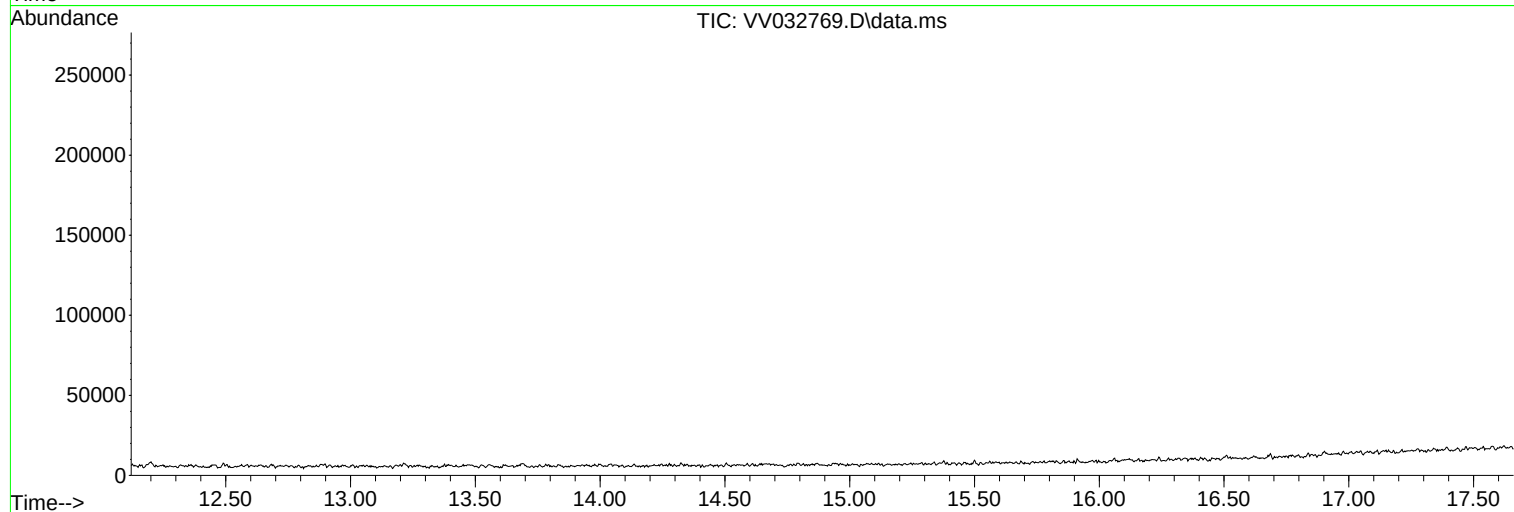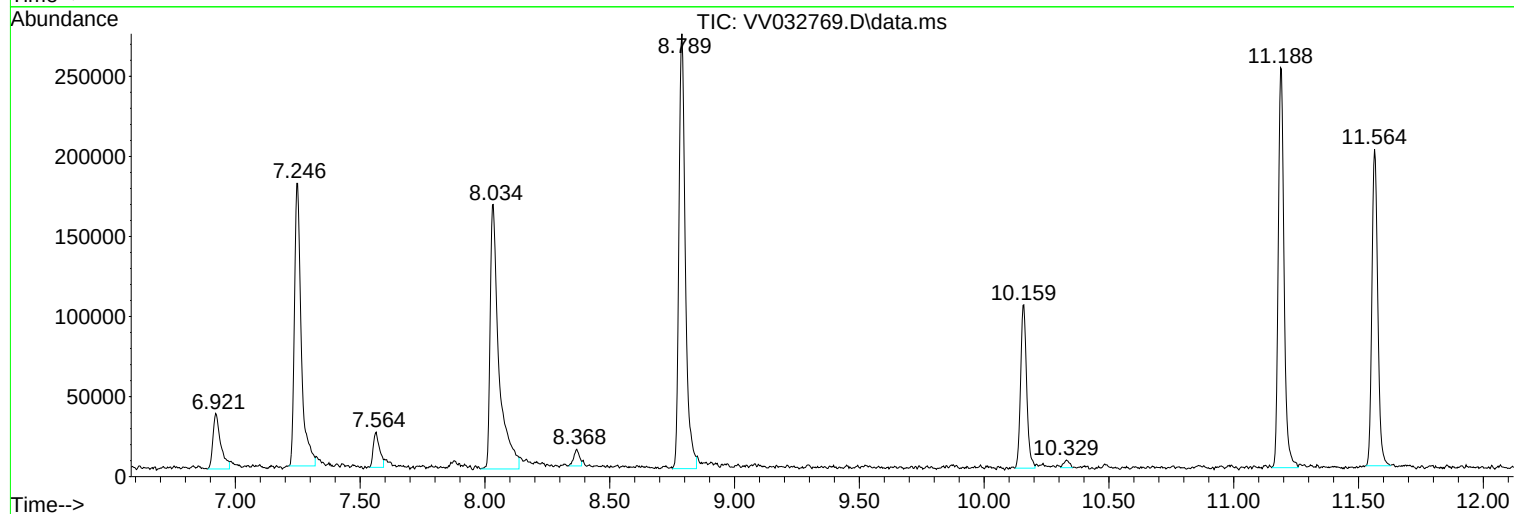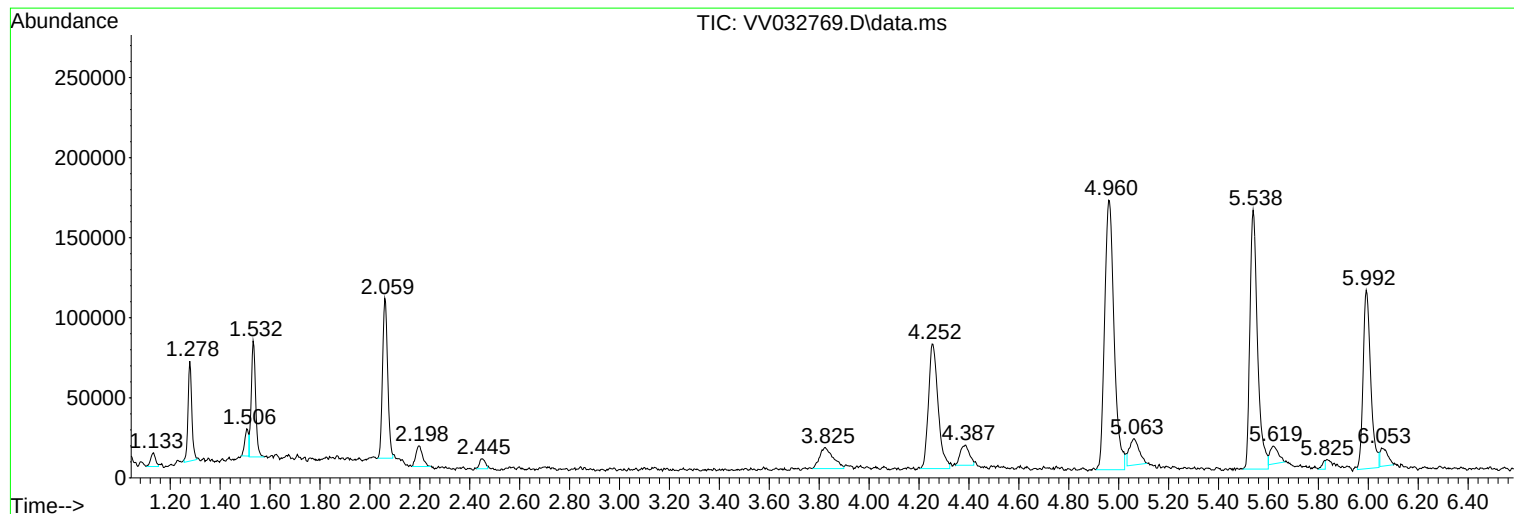

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032769.D
Acq On : 30 Oct 2023 14:04
Operator : SY/MD
Sample : 05019-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032769.D
Acq On : 30 Oct 2023 14:04
Operator : SY/MD
Sample : 05019-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc