

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
 Data File : VV032775.D
 Acq On : 30 Oct 2023 16:31
 Operator : SY/MD
 Sample : 05019-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032775.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	20	26	37	rVB	11867	16401	3.29%	0.372%
2	1.278	66	74	86	rBV	70572	78280	15.72%	1.778%
3	1.532	147	153	161	rBV	65008	74518	14.96%	1.692%
4	2.060	305	317	329	rBV	121006	179192	35.97%	4.069%
5	2.188	348	357	370	rVB2	17234	33677	6.76%	0.765%
6	3.828	855	867	891	rBV3	40865	175048	35.14%	3.975%
7	4.252	983	999	1021	rBV	80357	216403	43.45%	4.914%
8	4.375	1027	1037	1049	rBV3	9419	20700	4.16%	0.470%
9	4.960	1204	1219	1237	rBV3	184644	468467	94.05%	10.638%
10	5.059	1244	1250	1267	rVB4	14139	31535	6.33%	0.716%
11	5.538	1386	1399	1416	rBV	153784	326184	65.49%	7.407%
12	5.622	1418	1425	1433	rVB2	9397	18873	3.79%	0.429%
13	5.992	1528	1540	1554	rBV2	110894	235717	47.32%	5.353%
14	6.918	1819	1828	1843	rBV2	45916	93508	18.77%	2.123%
15	7.246	1917	1930	1956	rBV	205459	396735	79.65%	9.009%
16	7.561	2017	2028	2045	rBV	28441	56549	11.35%	1.284%
17	7.882	2116	2128	2136	rBV3	10606	20375	4.09%	0.463%
18	8.034	2165	2175	2210	rBV2	209378	498103	100.00%	11.311%
19	8.368	2271	2279	2288	rBV2	6332	12939	2.60%	0.294%
20	8.789	2399	2410	2434	rBV	263382	470919	94.54%	10.694%
21	10.156	2825	2835	2848	rBV	92930	152489	30.61%	3.463%
22	10.326	2880	2888	2899	rVB3	17562	31341	6.29%	0.712%
23	11.188	3145	3156	3175	rBV	260825	416026	83.52%	9.447%
24	11.564	3261	3273	3291	rBV	216487	353651	71.00%	8.031%
25	12.197	3459	3470	3480	rBV2	10830	19382	3.89%	0.440%
26	13.985	4018	4026	4032	rBV8	4170	6747	1.35%	0.153%




Sum of corrected areas: 4403759

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032775.D
Acq On : 30 Oct 2023 16:31
Operator : SY/MD
Sample : 05019-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

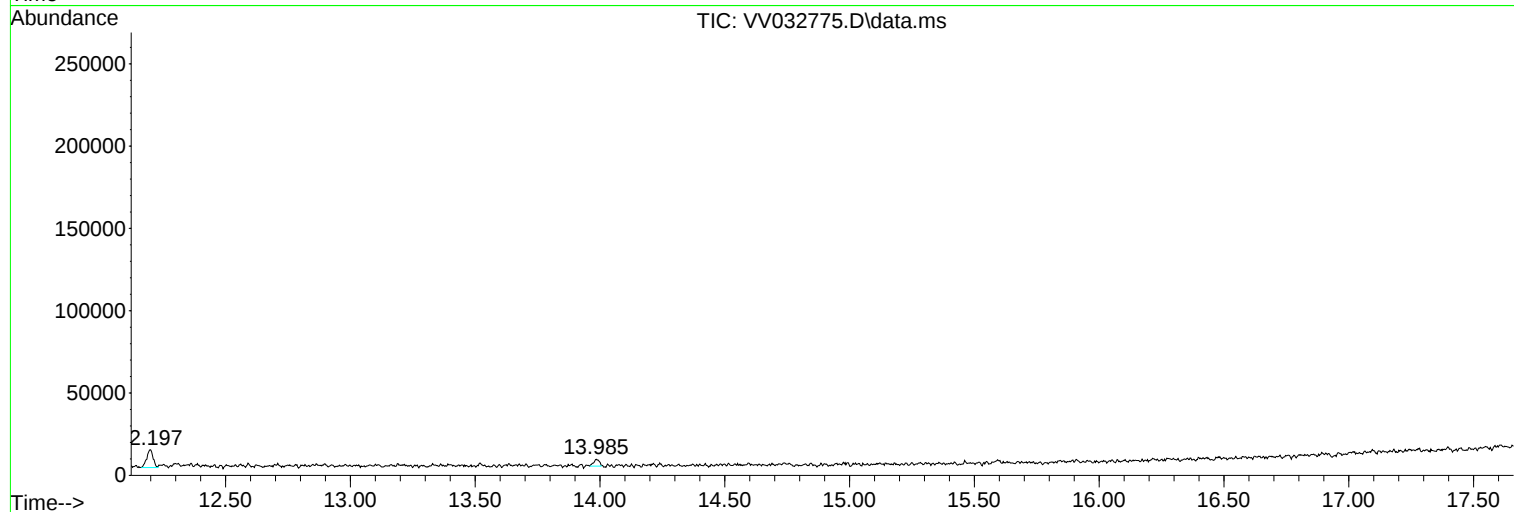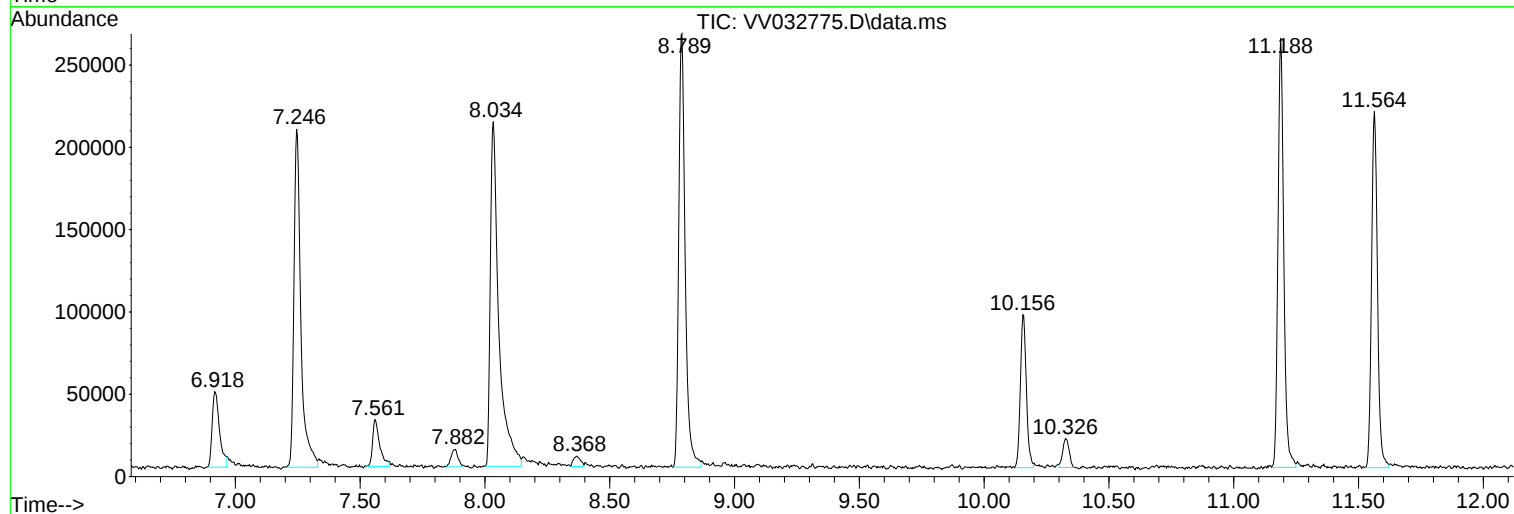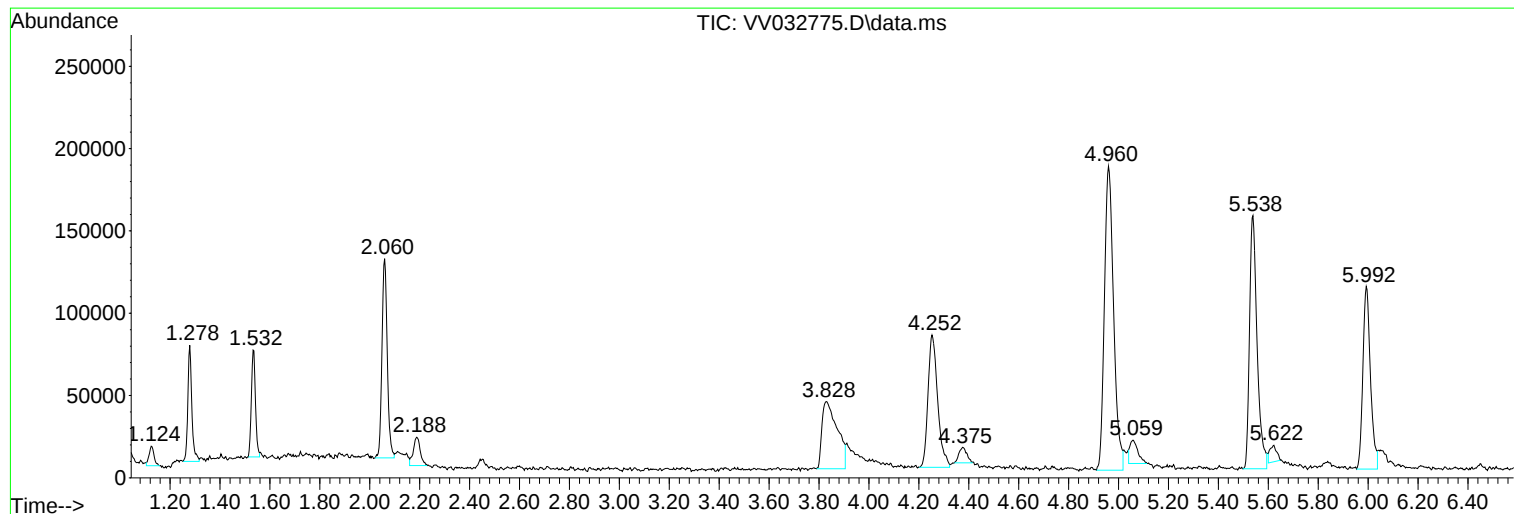

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032775.D
Acq On : 30 Oct 2023 16:31
Operator : SY/MD
Sample : 05019-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032775.D
Acq On : 30 Oct 2023 16:31
Operator : SY/MD
Sample : 05019-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------