

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
 Data File : VV032779.D
 Acq On : 30 Oct 2023 18:08
 Operator : SY/MD
 Sample : 05114-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B65

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032779.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.121	18	25	33	rVB	25619	32619	6.49%	0.747%
2	1.278	66	74	85	rBV	63863	71014	14.12%	1.627%
3	1.388	101	108	116	rBV	18484	23423	4.66%	0.537%
4	1.532	147	153	163	rVB	62427	71745	14.27%	1.644%
5	2.060	307	317	332	rBV	113026	167116	33.24%	3.829%
6	2.127	334	338	348	rVV8	5189	7244	1.44%	0.166%
7	2.185	348	356	366	rVB	13447	22985	4.57%	0.527%
8	2.606	476	487	490	rBV6	6511	11608	2.31%	0.266%
9	3.806	846	860	889	rBV4	75081	272024	54.10%	6.232%
10	4.253	984	999	1022	rBV2	79668	218246	43.41%	5.000%
11	4.375	1027	1037	1039	rBV3	8062	11922	2.37%	0.273%
12	4.960	1203	1219	1239	rBV2	175579	453531	90.20%	10.390%
13	5.050	1244	1247	1267	rVB5	14534	32997	6.56%	0.756%
14	5.539	1387	1399	1417	rBV	145622	313130	62.28%	7.174%
15	5.992	1525	1540	1556	rBV	108007	226212	44.99%	5.182%
16	6.918	1817	1828	1842	rBV2	44254	89027	17.71%	2.040%
17	7.246	1920	1930	1955	rVV	188617	366642	72.92%	8.400%
18	7.561	2019	2028	2044	rBV2	27701	55722	11.08%	1.277%
19	7.873	2118	2125	2140	rBV4	12689	27614	5.49%	0.633%
20	8.031	2164	2174	2208	rBV	229849	502800	100.00%	11.519%
21	8.786	2399	2409	2431	rBV	252795	452070	89.91%	10.357%
22	10.156	2822	2835	2850	rBV2	90823	153988	30.63%	3.528%
23	10.329	2876	2889	2900	rVB4	22722	38147	7.59%	0.874%
24	11.188	3145	3156	3172	rBV	249415	387138	77.00%	8.869%
25	11.564	3261	3273	3290	rBV	207678	335309	66.69%	7.682%
26	12.201	3461	3471	3479	rBV2	7922	14388	2.86%	0.330%
27	13.985	4019	4026	4030	rBV8	4705	6370	1.27%	0.146%




Sum of corrected areas: 4365031

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032779.D
Acq On : 30 Oct 2023 18:08
Operator : SY/MD
Sample : 05114-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

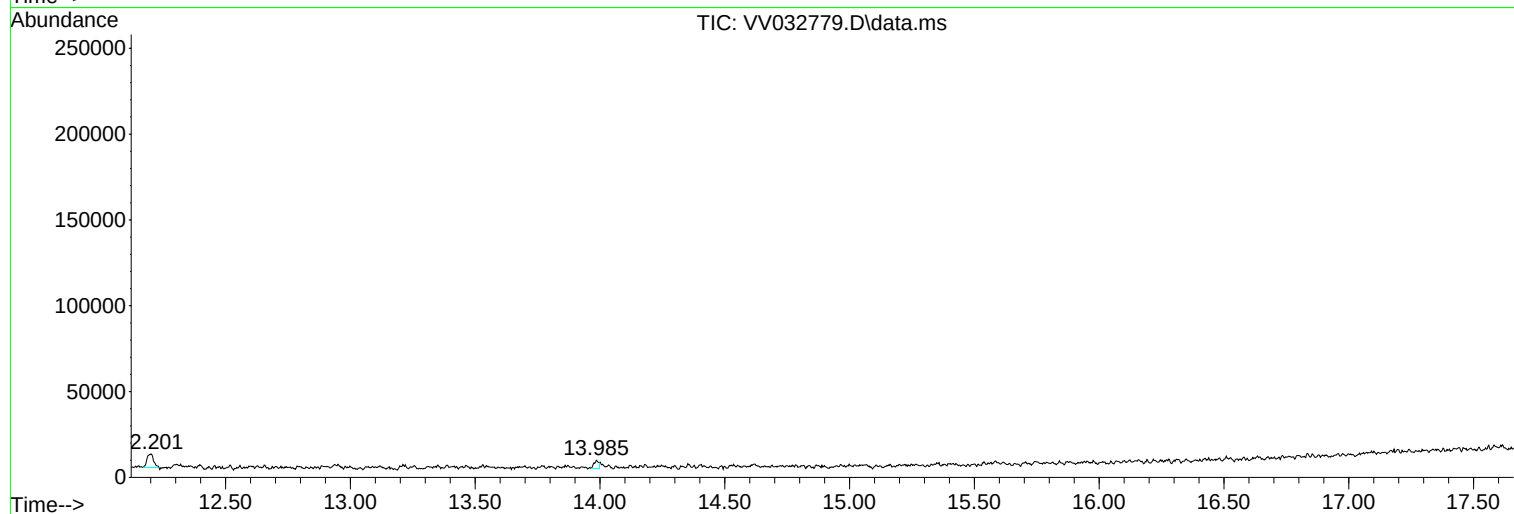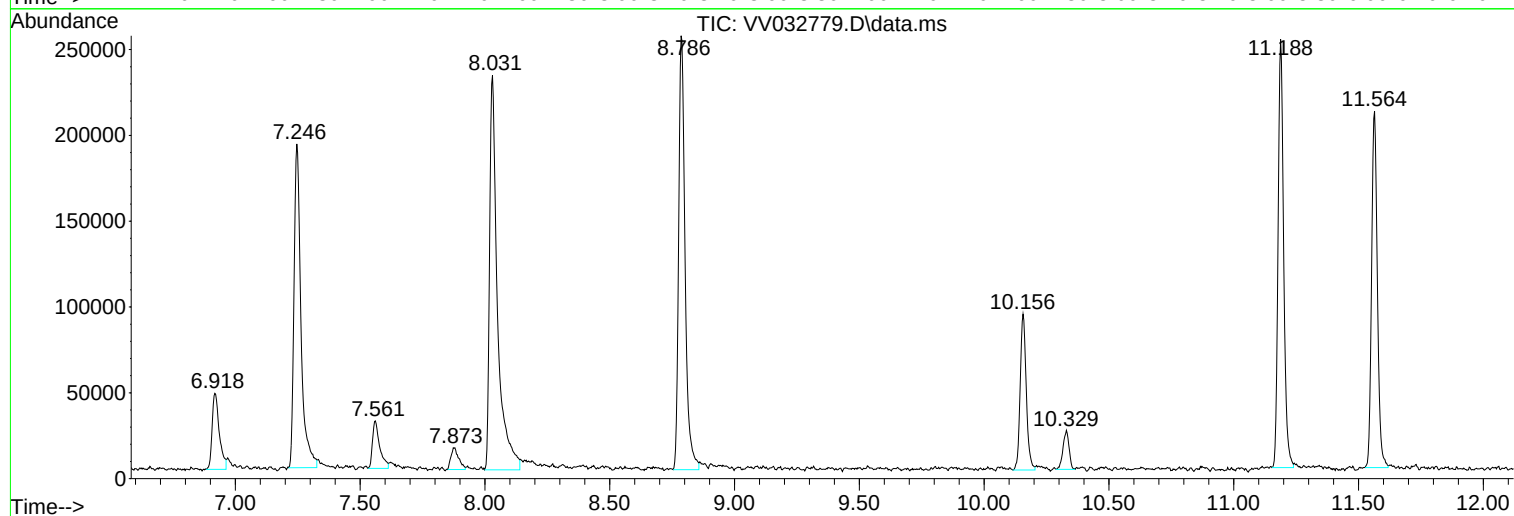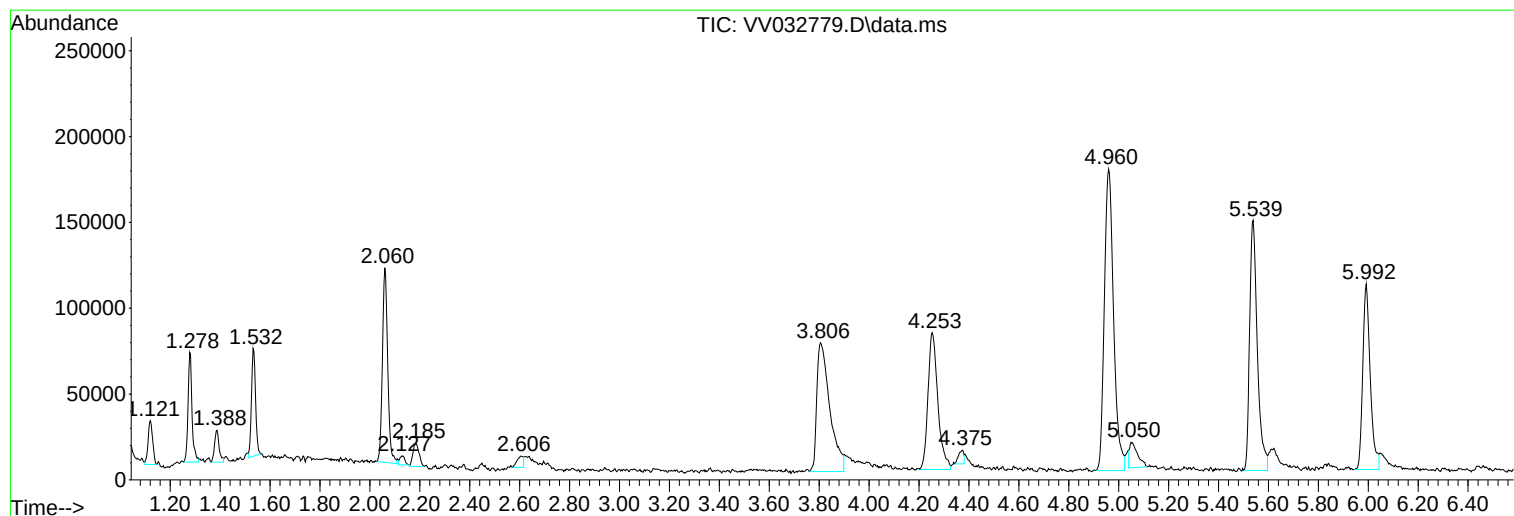

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032779.D
Acq On : 30 Oct 2023 18:08
Operator : SY/MD
Sample : 05114-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032779.D
Acq On : 30 Oct 2023 18:08
Operator : SY/MD
Sample : 05114-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc