

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
 Data File : VV032780.D
 Acq On : 30 Oct 2023 18:32
 Operator : SY/MD
 Sample : 05114-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B66

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032780.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	17	24	33	rVB	17586	23383	4.83%	0.561%
2	1.278	67	74	92	rVB	65323	74546	15.38%	1.790%
3	1.532	147	153	166	rVB	63484	73016	15.07%	1.753%
4	2.060	306	317	334	rVV	108718	163550	33.75%	3.927%
5	2.182	346	355	366	rVB3	15400	26746	5.52%	0.642%
6	2.452	431	439	450	rVB3	5225	7991	1.65%	0.192%
7	2.609	473	488	493	rBV4	9740	22676	4.68%	0.545%
8	3.802	848	859	881	rBV2	55847	183899	37.95%	4.416%
9	4.252	983	999	1024	rBV2	77570	216810	44.74%	5.206%
10	4.375	1026	1037	1054	rVB3	10418	32057	6.62%	0.770%
11	4.960	1204	1219	1237	rBV3	173528	440846	90.98%	10.586%
12	5.539	1388	1399	1418	rBV2	134571	286805	59.19%	6.887%
13	5.616	1418	1423	1435	rVB5	10207	19951	4.12%	0.479%
14	5.992	1527	1540	1556	rBV2	103671	223268	46.08%	5.361%
15	6.918	1815	1828	1855	rBV	46109	101183	20.88%	2.430%
16	7.246	1918	1930	1956	rBV	191860	375318	77.46%	9.012%
17	7.561	2020	2028	2045	rBV	25686	50920	10.51%	1.223%
18	7.876	2116	2126	2134	rBV2	13022	24618	5.08%	0.591%
19	8.030	2164	2174	2208	rBV	219539	484550	100.00%	11.635%
20	8.789	2398	2410	2430	rBV	234386	412666	85.16%	9.909%
21	9.532	2637	2641	2647	rVB	7451	6043	1.25%	0.145%
22	10.156	2823	2835	2856	rBV	93040	158431	32.70%	3.804%
23	10.326	2878	2888	2900	rBV2	26903	45910	9.47%	1.102%
24	11.188	3146	3156	3172	rBV	227642	359320	74.16%	8.628%
25	11.564	3261	3273	3285	rBV	205981	328445	67.78%	7.887%
26	12.194	3463	3469	3479	rVB4	10417	16324	3.37%	0.392%
27	13.988	4024	4027	4035	rVB8	5107	5178	1.07%	0.124%




Sum of corrected areas: 4164450

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032780.D
Acq On : 30 Oct 2023 18:32
Operator : SY/MD
Sample : 05114-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

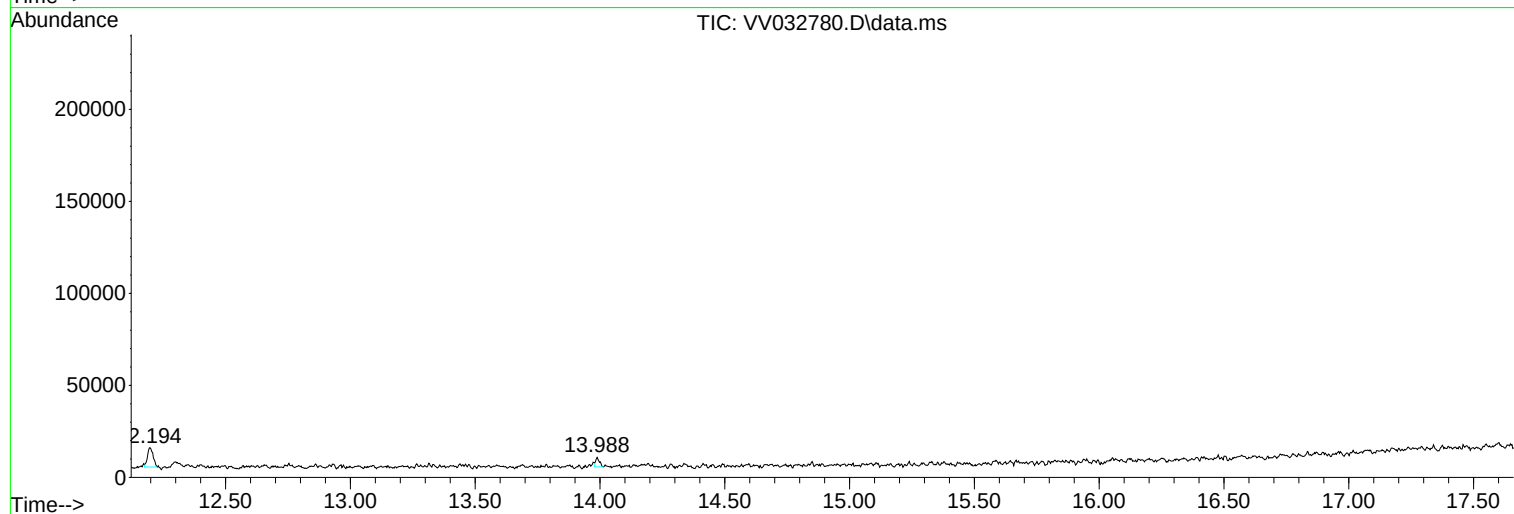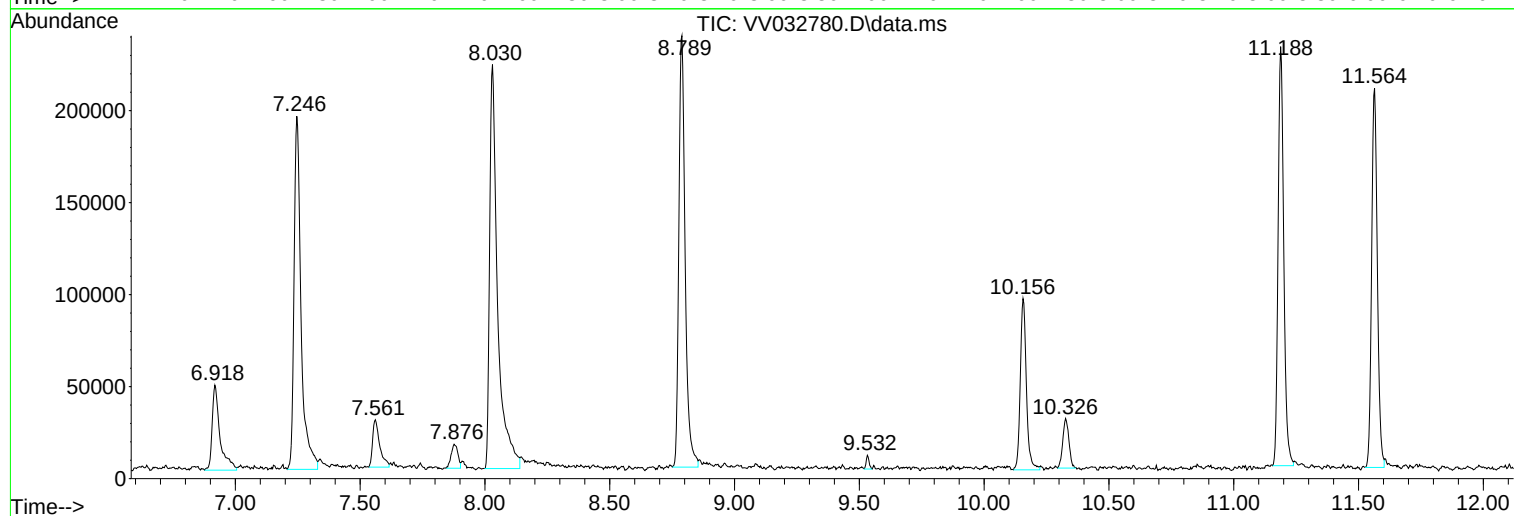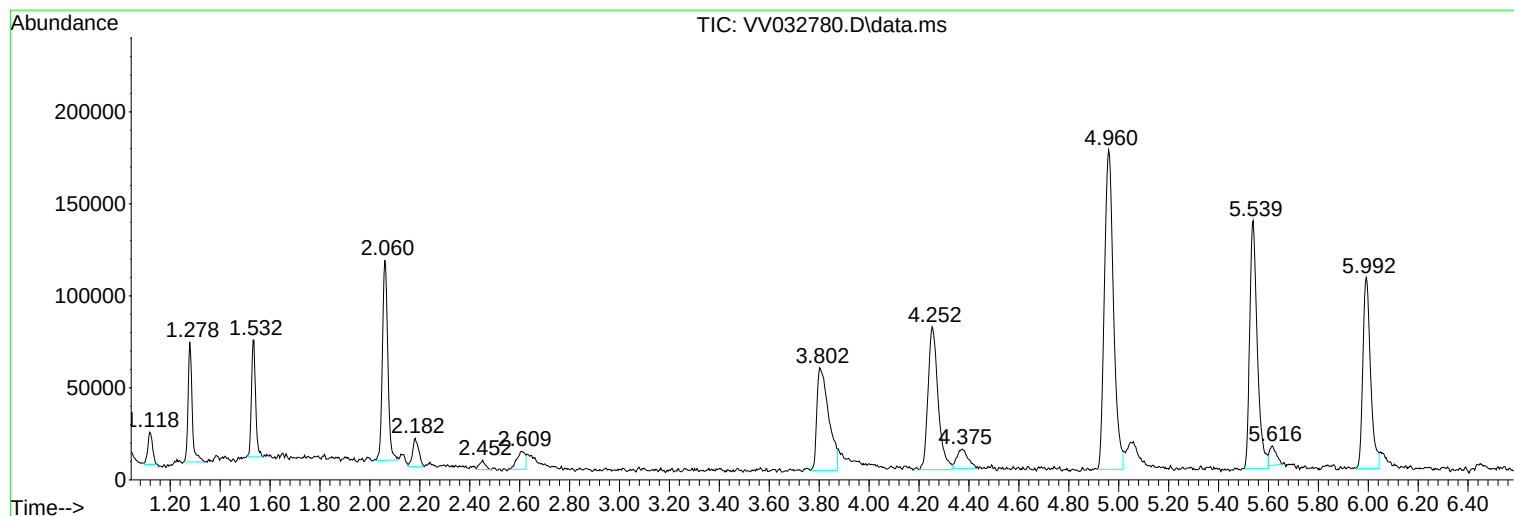

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032780.D
Acq On : 30 Oct 2023 18:32
Operator : SY/MD
Sample : 05114-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032780.D
Acq On : 30 Oct 2023 18:32
Operator : SY/MD
Sample : 05114-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc