


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103023\
Data File : VV032757.D
Acq On : 30 Oct 2023 08:23
Operator : SY/MD
Sample : BFB230
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB230

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Oct 31 02:23:31 2023

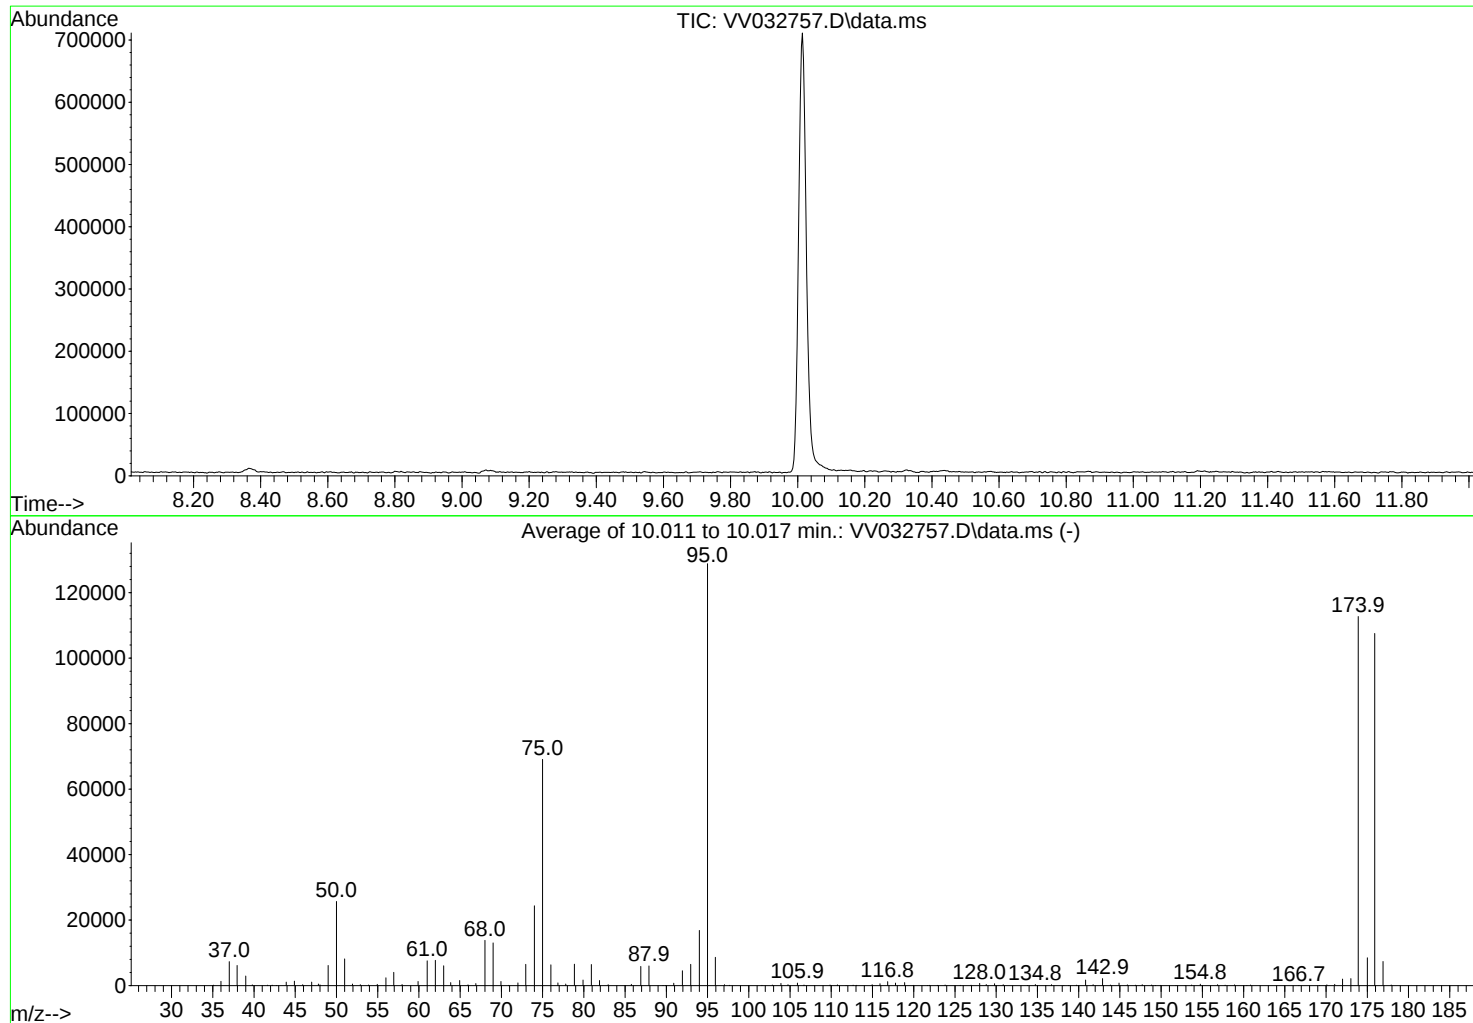

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	25680	PASS
75	95	30	80	53.6	69064	PASS
95	95	100	100	100.0	128835	PASS
96	95	5	9	6.7	8644	PASS
173	174	0.00	2	1.9	2125	PASS
174	95	50	120	87.5	112744	PASS
175	174	5	9	7.5	8501	PASS
176	174	95	105	95.4	107525	PASS
177	176	5	10	6.8	7344	PASS

m/z	Abundance
35.70	191.0
36.40	166.0
37.30	137.0
38.00	162.0
39.80	277.0
40.50	186.0
41.00	145.0
42.70	124.0
43.10	119.0
43.80	478.0
45.60	130.0
47.20	166.0
49.00	178.0
51.40	107.0
52.20	105.0
52.90	106.0
54.40	107.0
56.30	125.0
58.60	126.0
60.00	135.0
63.80	120.0
65.50	114.0
68.10	102.0
75.70	146.0
76.90	172.0
78.80	144.0
82.00	158.0
83.30	109.0
85.10	102.0
88.90	102.0
91.70	107.0
95.90	109.0
107.90	112.0
111.80	114.0
147.70	101.0
206.90	107.0
268.40	180.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

m/z	Abundance
35.10	175.0
36.00	1440.0
37.00	7625.0
38.00	6452.0
39.00	2972.0
39.80	505.0
41.70	164.0
42.20	119.0
42.80	174.0
43.90	1462.0
44.90	1328.0
45.90	246.0
47.00	1271.0
47.80	710.0
49.00	6411.0
50.00	26344.0
51.00	8095.0
51.90	541.0
52.90	329.0
53.80	154.0
55.00	416.0
56.00	2341.0
56.90	4209.0
58.00	287.0
59.90	1413.0
61.00	7634.0
62.00	7920.0
63.00	6230.0
63.90	1134.0
64.90	1649.0
66.00	222.0
66.90	560.0
68.00	14118.0
69.00	13525.0
70.00	1349.0
72.00	807.0
73.00	6649.0
74.00	24944.0
75.00	70152.0
76.00	6201.0
76.80	882.0
77.80	379.0
78.90	7070.0
79.90	1671.0
80.90	6650.0
81.90	1705.0
82.90	229.0
85.00	115.0
85.70	396.0
86.90	5941.0
87.90	6253.0
89.60	122.0
89.90	126.0
90.90	695.0
91.90	4654.0
92.90	6542.0
94.00	17448.0
95.00	129472.0
96.00	8892.0
97.10	281.0
102.90	194.0
103.90	700.0
104.70	248.0
105.90	805.0
106.80	152.0
108.10	112.0
109.80	173.0
110.80	254.0
111.80	133.0
112.70	145.0
114.90	265.0
115.90	527.0
116.80	1204.0
117.80	725.0
118.90	921.0
119.90	158.0
121.70	118.0
122.90	104.0
123.80	163.0
125.70	123.0
127.00	102.0
128.00	581.0
128.80	319.0
129.80	574.0
130.90	264.0
133.80	140.0
134.70	280.0
136.70	302.0
138.80	114.0
139.80	141.0
140.90	1609.0
141.70	274.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

142.90	2197.0
143.80	160.0
144.90	720.0
145.80	227.0
146.90	146.0
147.80	368.0
149.00	196.0
149.90	122.0
151.80	106.0
153.70	197.0
154.80	394.0
156.90	314.0
157.80	166.0
158.90	190.0
160.80	194.0
169.20	110.0
170.10	149.0
171.00	394.0
172.00	1752.0
173.00	2021.0
173.90	109224.0
175.00	8230.0
175.90	105128.0
176.90	7158.0
177.90	196.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

m/z	Abundance
36.00	1348.0
37.00	7613.0
38.00	6524.0
39.00	2987.0
39.80	491.0
41.60	155.0
42.20	129.0
42.80	149.0
44.00	1535.0
44.90	1360.0
45.90	235.0
47.00	1199.0
47.80	700.0
49.00	6507.0
50.00	26480.0
51.00	8377.0
52.00	500.0
52.90	425.0
53.90	139.0
54.90	392.0
56.00	2424.0
56.90	4187.0
57.90	317.0
59.90	1372.0
61.00	7832.0
62.00	8034.0
63.00	6183.0
63.90	1092.0
64.90	1626.0
65.90	222.0
66.90	639.0
68.00	14258.0
69.00	13330.0
69.90	1300.0
70.90	135.0
72.00	816.0
73.00	6690.0
74.00	25152.0
75.00	71240.0
76.00	6618.0
76.90	972.0
77.80	496.0
78.90	6866.0
79.90	1729.0
80.90	6576.0
81.90	1761.0
83.00	258.0
85.00	124.0
85.70	387.0
86.90	6045.0
87.90	6219.0
90.90	734.0
91.90	4628.0
93.00	6665.0
94.00	17384.0
95.00	133184.0
96.00	9007.0
97.00	267.0
97.60	143.0
101.60	108.0
102.90	179.0
103.90	664.0
104.80	264.0
105.90	766.0
106.70	163.0
108.00	160.0
109.90	181.0
110.80	248.0
111.80	156.0
112.60	154.0
113.00	131.0
115.00	306.0
115.90	576.0
116.80	1259.0
117.80	768.0
118.90	962.0
120.00	136.0
121.90	121.0
122.90	102.0
123.80	177.0
125.60	116.0
127.00	110.0
128.00	685.0
128.80	353.0
129.80	587.0
130.90	293.0
134.70	333.0
136.70	257.0
139.80	148.0
140.80	1714.0
141.80	268.0
142.90	2186.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

143.90	206.0
144.90	774.0
145.90	226.0
146.90	125.0
147.80	413.0
148.80	154.0
149.30	109.0
150.00	114.0
153.70	178.0
154.80	431.0
156.80	287.0
157.80	156.0
158.90	208.0
160.80	186.0
170.10	227.0
171.10	386.0
172.00	2082.0
173.00	2263.0
173.90	116368.0
175.00	8772.0
175.90	111184.0
176.90	7599.0
177.90	200.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

m/z	Abundance
35.10	195.0
36.00	1122.0
37.00	6733.0
37.90	5922.0
39.00	2765.0
39.90	487.0
41.60	115.0
42.20	149.0
42.80	138.0
44.00	1542.0
44.90	1297.0
45.90	265.0
47.00	1149.0
48.00	727.0
49.00	6037.0
50.00	24216.0
51.00	7907.0
52.00	443.0
52.90	437.0
54.00	184.0
54.90	376.0
56.00	2352.0
57.00	3791.0
57.90	338.0
59.90	1303.0
61.00	7125.0
62.00	7180.0
63.00	5714.0
63.90	930.0
65.00	1349.0
65.90	274.0
66.90	633.0
68.00	13323.0
69.00	12275.0
69.90	1180.0
70.90	155.0
72.00	733.0
72.90	6087.0
74.00	22968.0
75.00	65800.0
76.00	6193.0
76.90	1023.0
77.80	582.0
78.90	6042.0
79.90	1642.0
80.90	6034.0
81.90	1612.0
83.00	292.0
85.00	106.0
85.80	341.0
86.90	5550.0
87.90	5483.0
90.90	736.0
92.00	4285.0
93.00	6286.0
94.00	15624.0
95.00	123848.0
96.00	8361.0
97.00	254.0
97.70	116.0
101.60	122.0
102.80	127.0
103.90	632.0
104.80	279.0
105.90	693.0
106.60	156.0
108.00	172.0
109.90	169.0
110.70	199.0
111.80	174.0
112.60	147.0
113.10	108.0
115.00	297.0
115.90	626.0
116.90	1099.0
117.80	720.0
118.90	840.0
121.90	128.0
123.80	153.0
126.90	120.0
128.00	684.0
128.80	297.0
129.80	557.0
130.80	288.0
134.80	363.0
136.00	124.0
136.70	184.0
138.20	100.0
139.70	127.0
140.80	1756.0
141.80	250.0
142.90	2062.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

143.80	193.0
144.90	774.0
146.00	200.0
146.90	117.0
147.70	374.0
148.70	151.0
152.90	104.0
153.70	126.0
154.70	374.0
156.80	252.0
157.70	123.0
158.90	213.0
160.40	140.0
160.90	147.0
166.70	103.0
170.10	224.0
171.10	338.0
172.00	2114.0
173.00	2092.0
173.90	112640.0
175.00	8502.0
175.90	106264.0
176.90	7275.0
177.90	163.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230