


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV103118\
Data File : VV008491.D
Acq On : 31 Oct 2018 12:57
Operator : SY/MD
Sample : BFB54
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB54

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM103118WMA.M
Title : VOC Analysis
Last Update : Thu Nov 01 09:14:28 2018

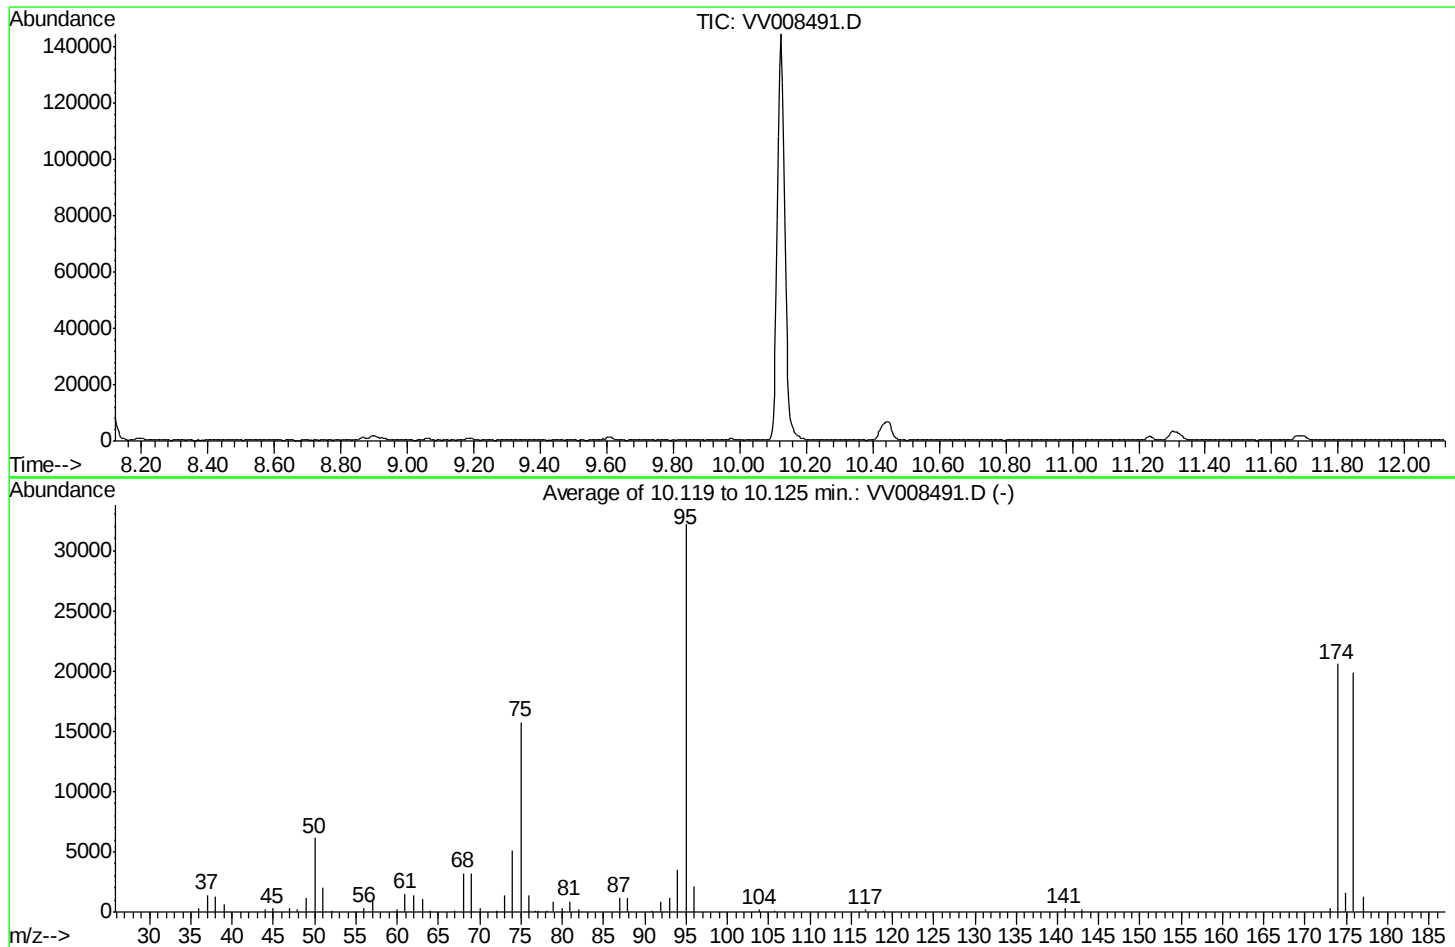

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	6111	PASS
75	95	30	80	49.0	15758	PASS
95	95	100	100	100.0	32162	PASS
96	95	5	9	6.7	2163	PASS
173	174	0.00	2	1.3	276	PASS
174	95	50	120	64.0	20592	PASS
175	174	5	9	7.6	1564	PASS
176	174	95	101	96.7	19912	PASS
177	176	5	9	6.3	1263	PASS

Scan 2798 (10.087 min): VV008491.D
BFB54

m/z	Abundance
39.90	106.0
43.90	264.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

m/z	Abundance
35.80	288.0
37.00	1297.0
38.00	1211.0
39.00	593.0
39.90	126.0
44.00	468.0
44.90	244.0
46.90	314.0
47.90	131.0
49.00	1108.0
50.00	5894.0
51.00	1975.0
52.00	152.0
56.00	386.0
56.90	881.0
60.00	236.0
60.90	1411.0
61.90	1372.0
63.00	979.0
63.90	133.0
68.00	3019.0
69.00	3080.0
70.00	269.0
72.00	135.0
73.00	1381.0
74.00	4796.0
75.00	15200.0
76.00	1330.0
77.10	169.0
78.10	102.0
78.90	852.0
79.90	264.0
80.90	792.0
82.00	162.0
86.90	1183.0
87.90	1139.0
92.00	839.0
93.00	1184.0
94.00	3259.0
95.00	30264.0
96.00	2117.0
103.90	157.0
105.70	127.0
116.80	139.0
118.80	137.0
140.90	281.0
142.90	236.0
173.00	227.0
173.90	19336.0
174.90	1570.0
175.90	18208.0
177.00	1186.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

m/z	Abundance
35.80	297.0
37.00	1454.0
38.00	1278.0
39.00	647.0
39.90	118.0
44.00	444.0
44.90	270.0
46.90	356.0
47.90	168.0
49.00	1157.0
50.00	6327.0
51.00	2048.0
52.00	151.0
56.00	378.0
56.90	922.0
59.90	251.0
61.00	1589.0
61.90	1392.0
63.00	1060.0
63.90	135.0
67.00	111.0
68.00	3318.0
69.00	3260.0
70.00	289.0
72.00	138.0
73.00	1452.0
74.00	5218.0
75.00	16201.0
76.00	1437.0
76.70	167.0
77.10	165.0
78.10	103.0
78.90	869.0
79.90	297.0
80.90	881.0
81.90	190.0
86.90	1255.0
87.90	1165.0
90.80	107.0
91.90	891.0
93.00	1251.0
94.00	3624.0
95.00	33336.0
96.00	2247.0
103.90	173.0
105.70	156.0
116.80	181.0
118.90	147.0
140.90	282.0
142.90	250.0
173.00	292.0
173.90	21272.0
175.00	1619.0
175.90	20608.0
177.00	1309.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

m/z	Abundance
35.00	294.0
37.00	1457.0
38.00	1212.0
39.00	570.0
44.00	409.0
44.90	300.0
46.90	353.0
47.90	201.0
49.00	1142.0
50.00	6114.0
51.00	1941.0
52.00	123.0
54.90	104.0
56.00	363.0
57.00	838.0
60.00	269.0
61.00	1531.0
62.00	1342.0
63.00	1046.0
64.00	125.0
67.00	129.0
68.00	3265.0
69.00	3109.0
70.00	260.0
72.00	153.0
73.00	1353.0
74.00	5138.0
75.00	15873.0
76.00	1383.0
76.80	182.0
78.90	776.0
79.90	279.0
80.90	887.0
81.90	211.0
87.00	1151.0
87.90	1067.0
90.80	124.0
91.90	909.0
93.00	1231.0
94.00	3575.0
95.00	32888.0
96.00	2126.0
103.90	165.0
105.80	158.0
116.80	211.0
118.90	131.0
140.90	273.0
143.00	239.0
173.00	311.0
173.90	21168.0
175.00	1504.0
175.90	20920.0
177.00	1295.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54