

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV103119\
 Data File : VV013456.D
 Acq On : 31 Oct 2019 19:49
 Operator : SY/MD
 Sample : K5635-02
 Misc : 25.0ML/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BE9G7

Quant Time: Nov 01 06:00:14 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR103119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 01 05:32:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	329716	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	349362	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	187220	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	125147	5.16	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	103.20%
7) Chloroethane-d5	1.58	69	106462	5.26	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.20%
11) 1,1-Dichloroethene-d2	2.13	63	169506	3.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.00%
20) 2-Butanone-d5	3.92	46	413610	54.94	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.88%
24) Chloroform-d	4.40	84	279923	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.00%
26) 1,2-Dichloroethane-d4	5.08	65	153233	5.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.00%
32) Benzene-d6	5.10	84	563798	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.60%
36) 1,2-Dichloropropane-d6	6.12	67	181953	5.02	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.40%
41) Toluene-d8	7.36	98	470513	4.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.60%
43) trans-1,3-Dichloropropene-	7.66	79	61597	4.24	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.80%
46) 2-Hexanone-d5	8.13	63	235461	44.05	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.10%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	121336	4.36	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	197046	5.18	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.60%


Target Compounds					Ovalue
13) Acetone	2.18	43	3925	1.151 ug/L	46


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV103119\
Data File : VV013456.D
Acq On : 31 Oct 2019 19:49
Operator : SY/MD
Sample : K5635-02
Misc : 25.0ML/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BE9G7

Quant Time: Nov 01 06:00:14 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR103119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 01 05:32:11 2019
Response via : Initial Calibration

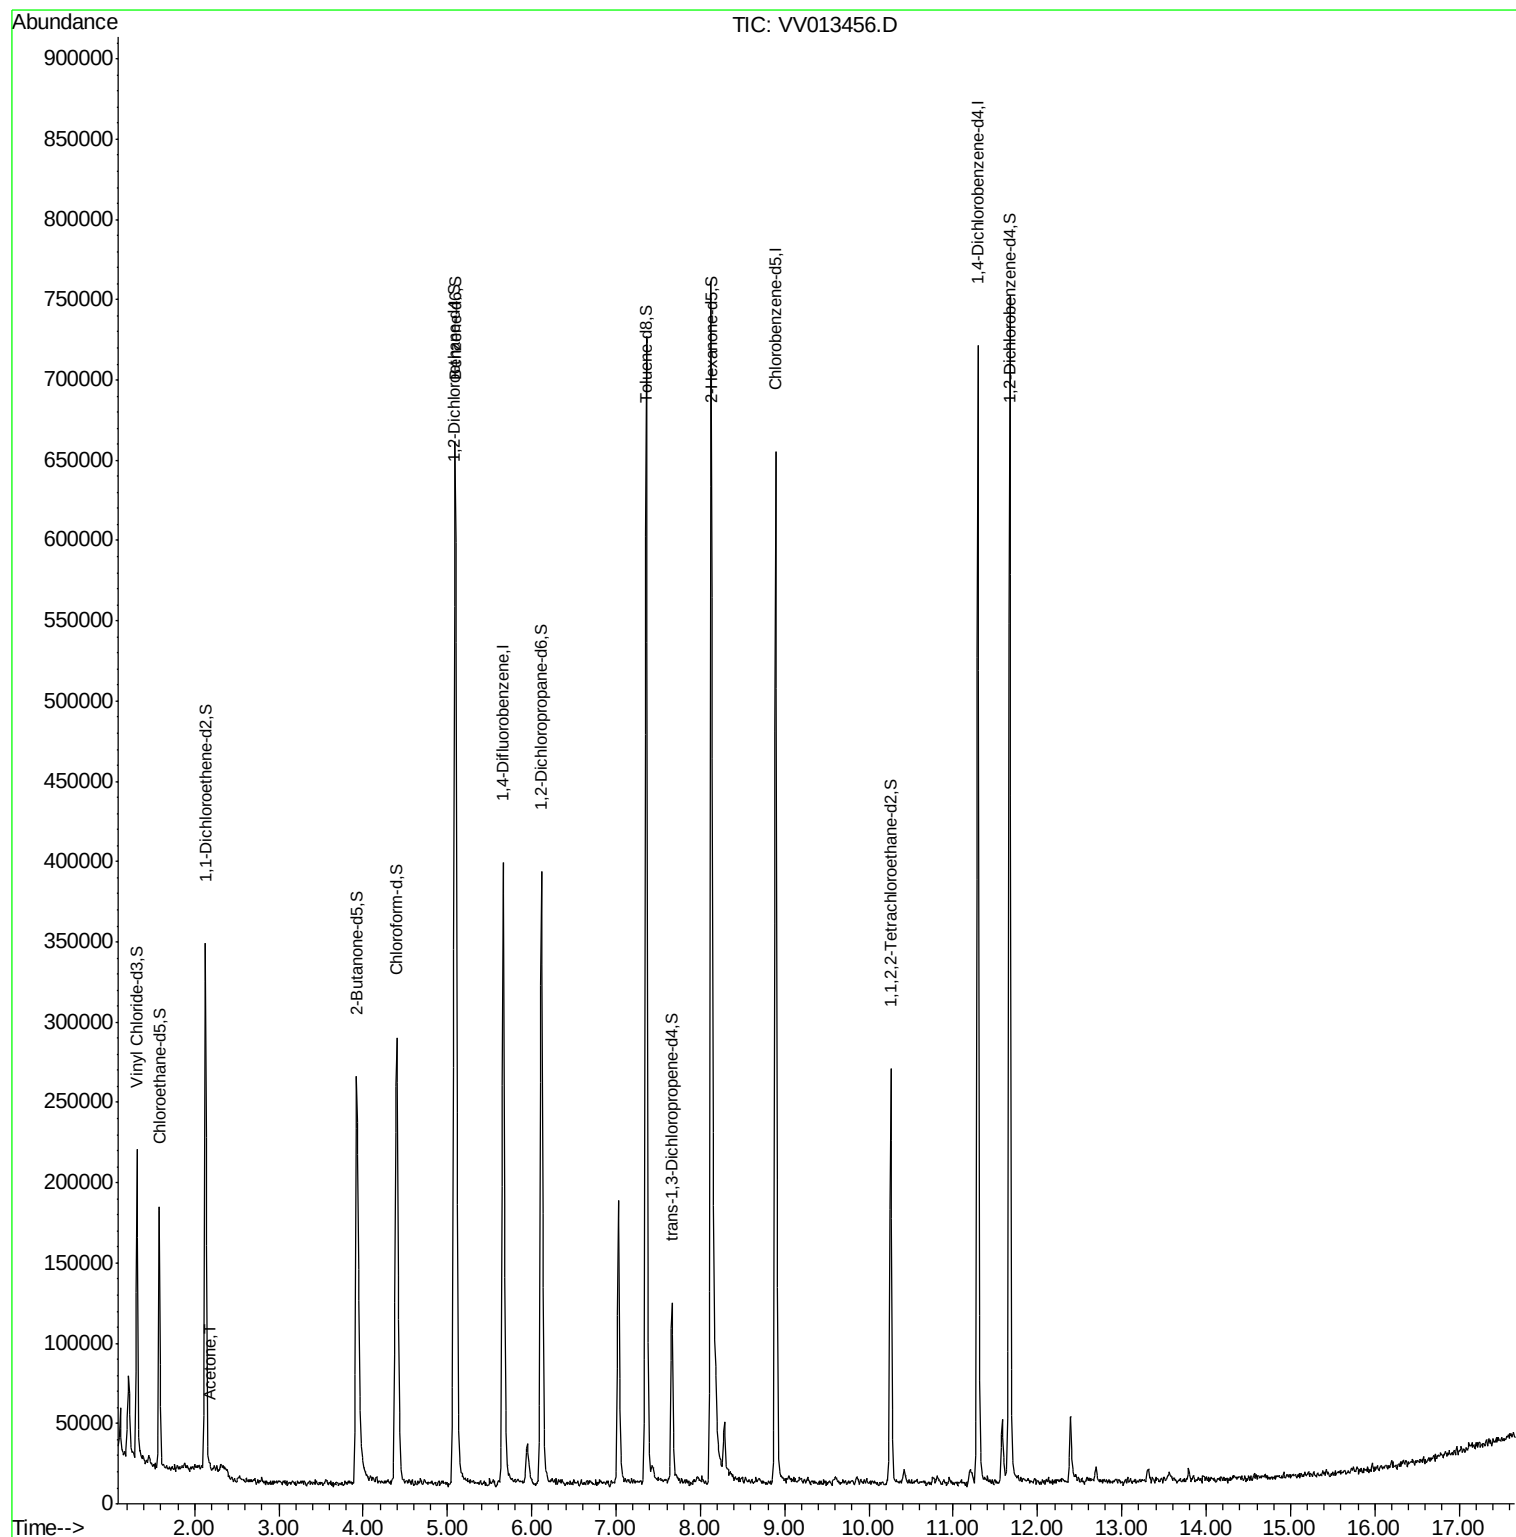

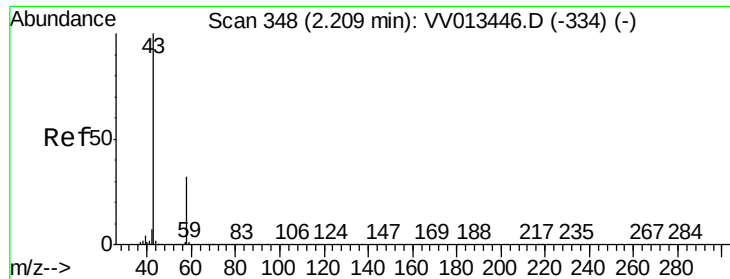

#13

Acetone

Concen: 1.151 ug/L

RT: 2.18 min Scan# 340

Delta R.T. -0.03 min

Lab File: VV013456.D

Acq: 31 Oct 2019 19:49

Instrument :

MSVOA_V

ClientSampleId :

BE9G7

Tot Ion: 43 Resp: 3925

Ion Ratio Lower Upper

43 100

58 57.6 0.0 58.0

