




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028779.D
 Acq On : 31 Oct 2022 14:33
 Operator : SY/MD
 Sample : VV1031WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK282

Manual IntegrationsAPPROVED

Quant Time: Nov 01 04:42:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 01 04:42:28 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 11/01/2022
 Supervised By :Mahesh Dadoda 11/01/2022

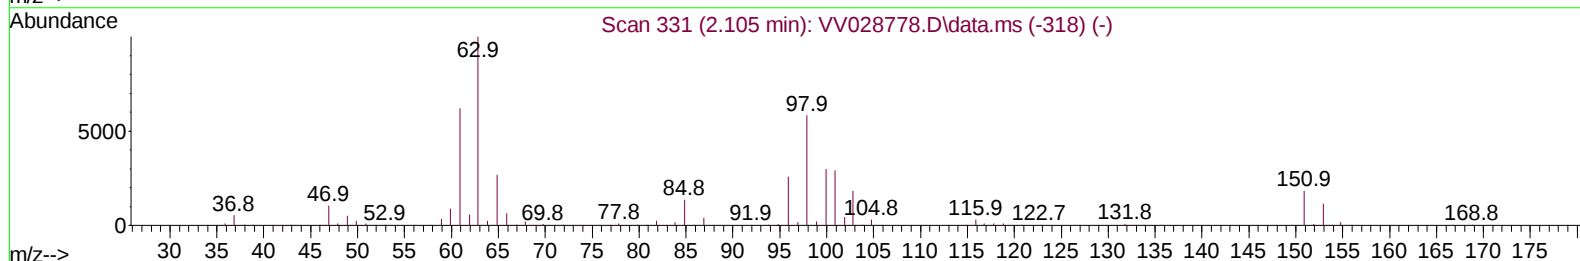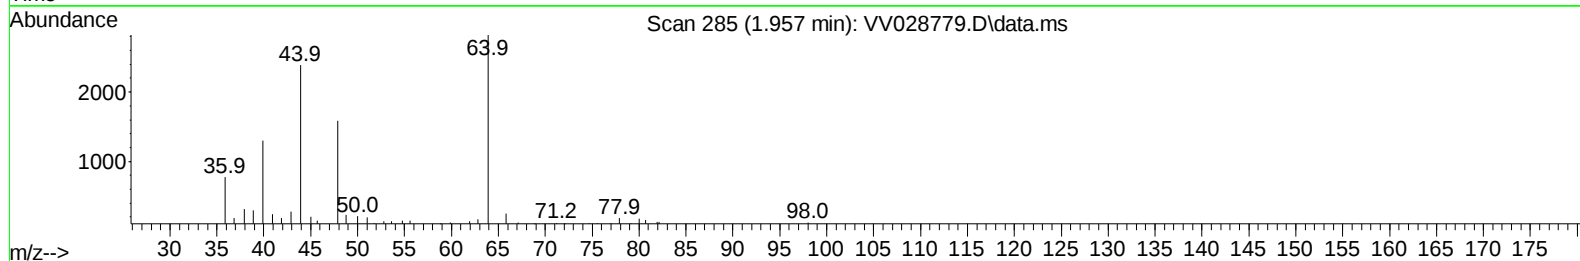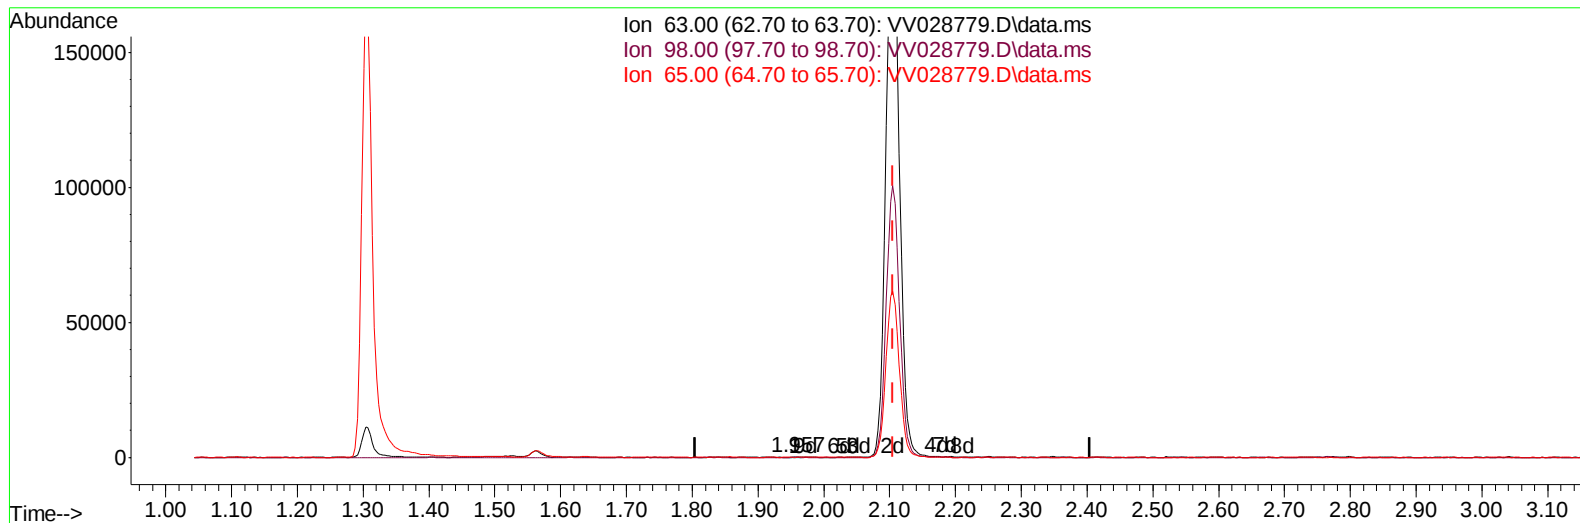

TIC: VV028779.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

1.957min (-0.148) 0.02 ug/L

response 156

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	62.00	43.59
65.00	23.30	27.56
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028779.D
 Acq On : 31 Oct 2022 14:33
 Operator : SY/MD
 Sample : VV1031WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK282

Manual IntegrationsAPPROVED

Quant Time: Nov 01 04:42:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 01 04:42:28 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 11/01/2022
 Supervised By :Mahesh Dadoda 11/01/2022

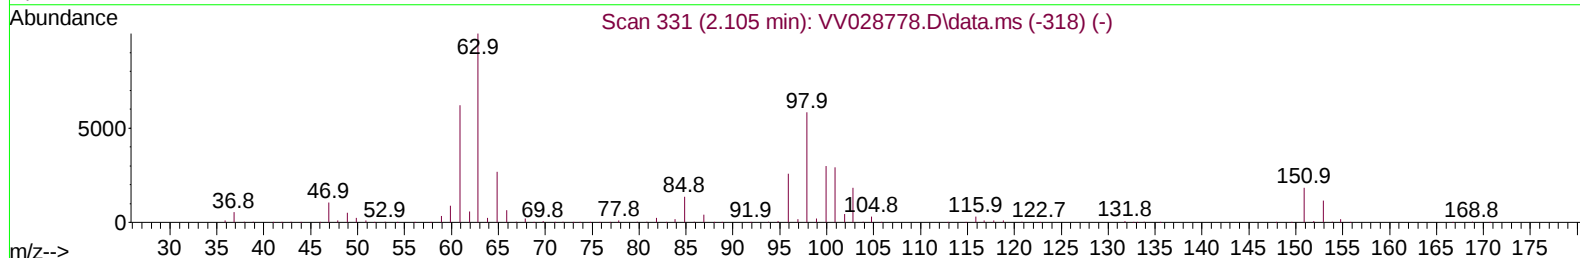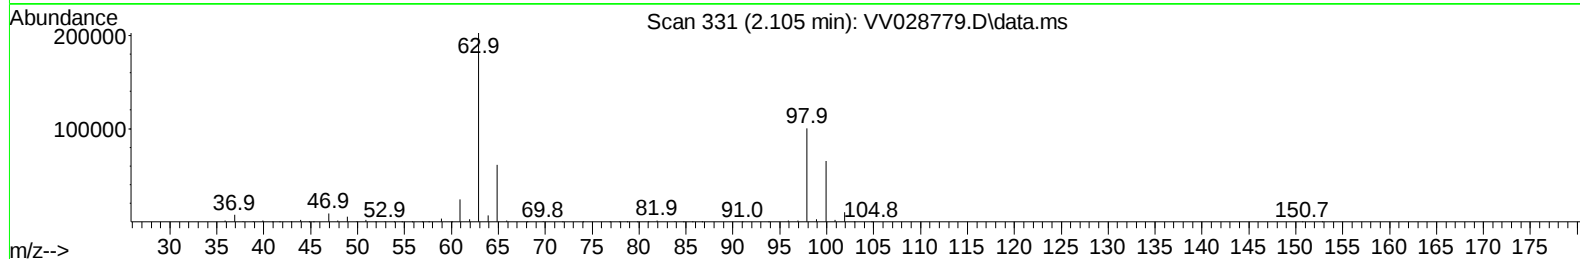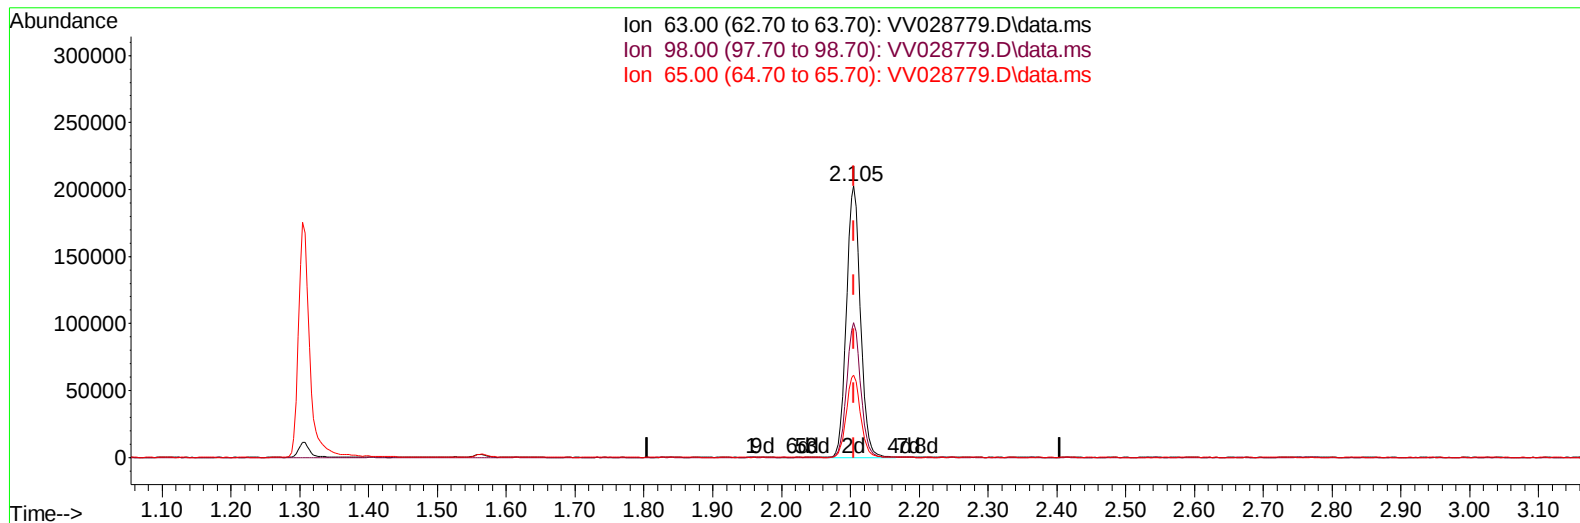

TIC: VV028779.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.105min (+ 0.000) 35.52 ug/L m

response 286711

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	62.00	0.02#
65.00	23.30	0.01#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028779.D
 Acq On : 31 Oct 2022 14:33
 Operator : SY/MD
 Sample : VV1031WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK282

Manual IntegrationsAPPROVED

Quant Time: Nov 01 04:42:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 01 04:42:28 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 11/01/2022
 Supervised By :Mahesh Dadoda 11/01/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	447640	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	401578	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	172421	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	198725	46.830	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	93.660%	
7) Chloroethane-d5	1.561	69	170151	46.905	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	93.800%	
11) 1,1-Dichloroethene-d2	2.105	63	286711m	35.519	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	71.040%	
21) 2-Butanone-d5	3.873	46	310241	100.434	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	100.430%	
24) Chloroform-d	4.343	84	292259	45.664	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	91.320%	
26) 1,2-Dichloroethane-d4	5.027	65	208290	49.208	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	98.420%	
32) Benzene-d6	5.043	84	630140	50.265	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	100.540%	
36) 1,2-Dichloropropane-d6	6.066	67	217043	50.429	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	100.860%	
41) Toluene-d8	7.310	98	536768	48.705	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	97.400%	
43) trans-1,3-Dichloroprop...	7.616	79	74211	44.894	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	89.780%	
47) 2-Hexanone-d5	8.085	63	186203	95.735	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	95.740%	
56) 1,1,2,2-Tetrachloroeth...	10.207	84	267419	47.119	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	94.240%	
66) 1,2-Dichlorobenzene-d4	11.616	152	168668	49.558	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	99.120%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028779.D
Acq On : 31 Oct 2022 14:33
Operator : SY/MD
Sample : VV1031WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK282

Manual IntegrationsAPPROVED

Quant Time: Nov 01 04:42:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 01 04:42:28 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 11/01/2022
Supervised By :Mahesh Dadoda 11/01/2022

