

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028791.D
 Acq On : 31 Oct 2022 19:31
 Operator : SY/MD
 Sample : N5354-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBMQ0

Quant Time: Nov 01 04:58:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 01 04:42:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	428368	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	382464	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	166152	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	128545	31.655	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	63.300%	
7) Chloroethane-d5	1.564	69	130113	37.481	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	74.960%	
11) 1,1-Dichloroethene-d2	2.105	63	202795	26.253	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	52.500%#	
21) 2-Butanone-d5	3.879	46	249382	84.364	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	84.360%	
24) Chloroform-d	4.342	84	241083	39.363	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	78.720%	
26) 1,2-Dichloroethane-d4	5.027	65	173083	42.730	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	85.460%	
32) Benzene-d6	5.047	84	497178	41.641	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	83.280%	
36) 1,2-Dichloropropane-d6	6.066	67	176326	43.016	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	86.040%	
41) Toluene-d8	7.310	98	422111	40.215	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	80.440%	
43) trans-1,3-Dichloroprop...	7.619	79	60142	38.202	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	76.400%	
47) 2-Hexanone-d5	8.085	63	151252	81.652	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	81.650%	
56) 1,1,2,2-Tetrachloroeth...	10.207	84	224960	41.619	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	83.240%	
66) 1,2-Dichlorobenzene-d4	11.615	152	141108	43.025	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	86.040%	
Target Compounds						
13) Acetone	2.169	43	22033	7.698	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028791.D
Acq On : 31 Oct 2022 19:31
Operator : SY/MD
Sample : N5354-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBMQ0

Quant Time: Nov 01 04:58:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 01 04:42:28 2022
Response via : Initial Calibration

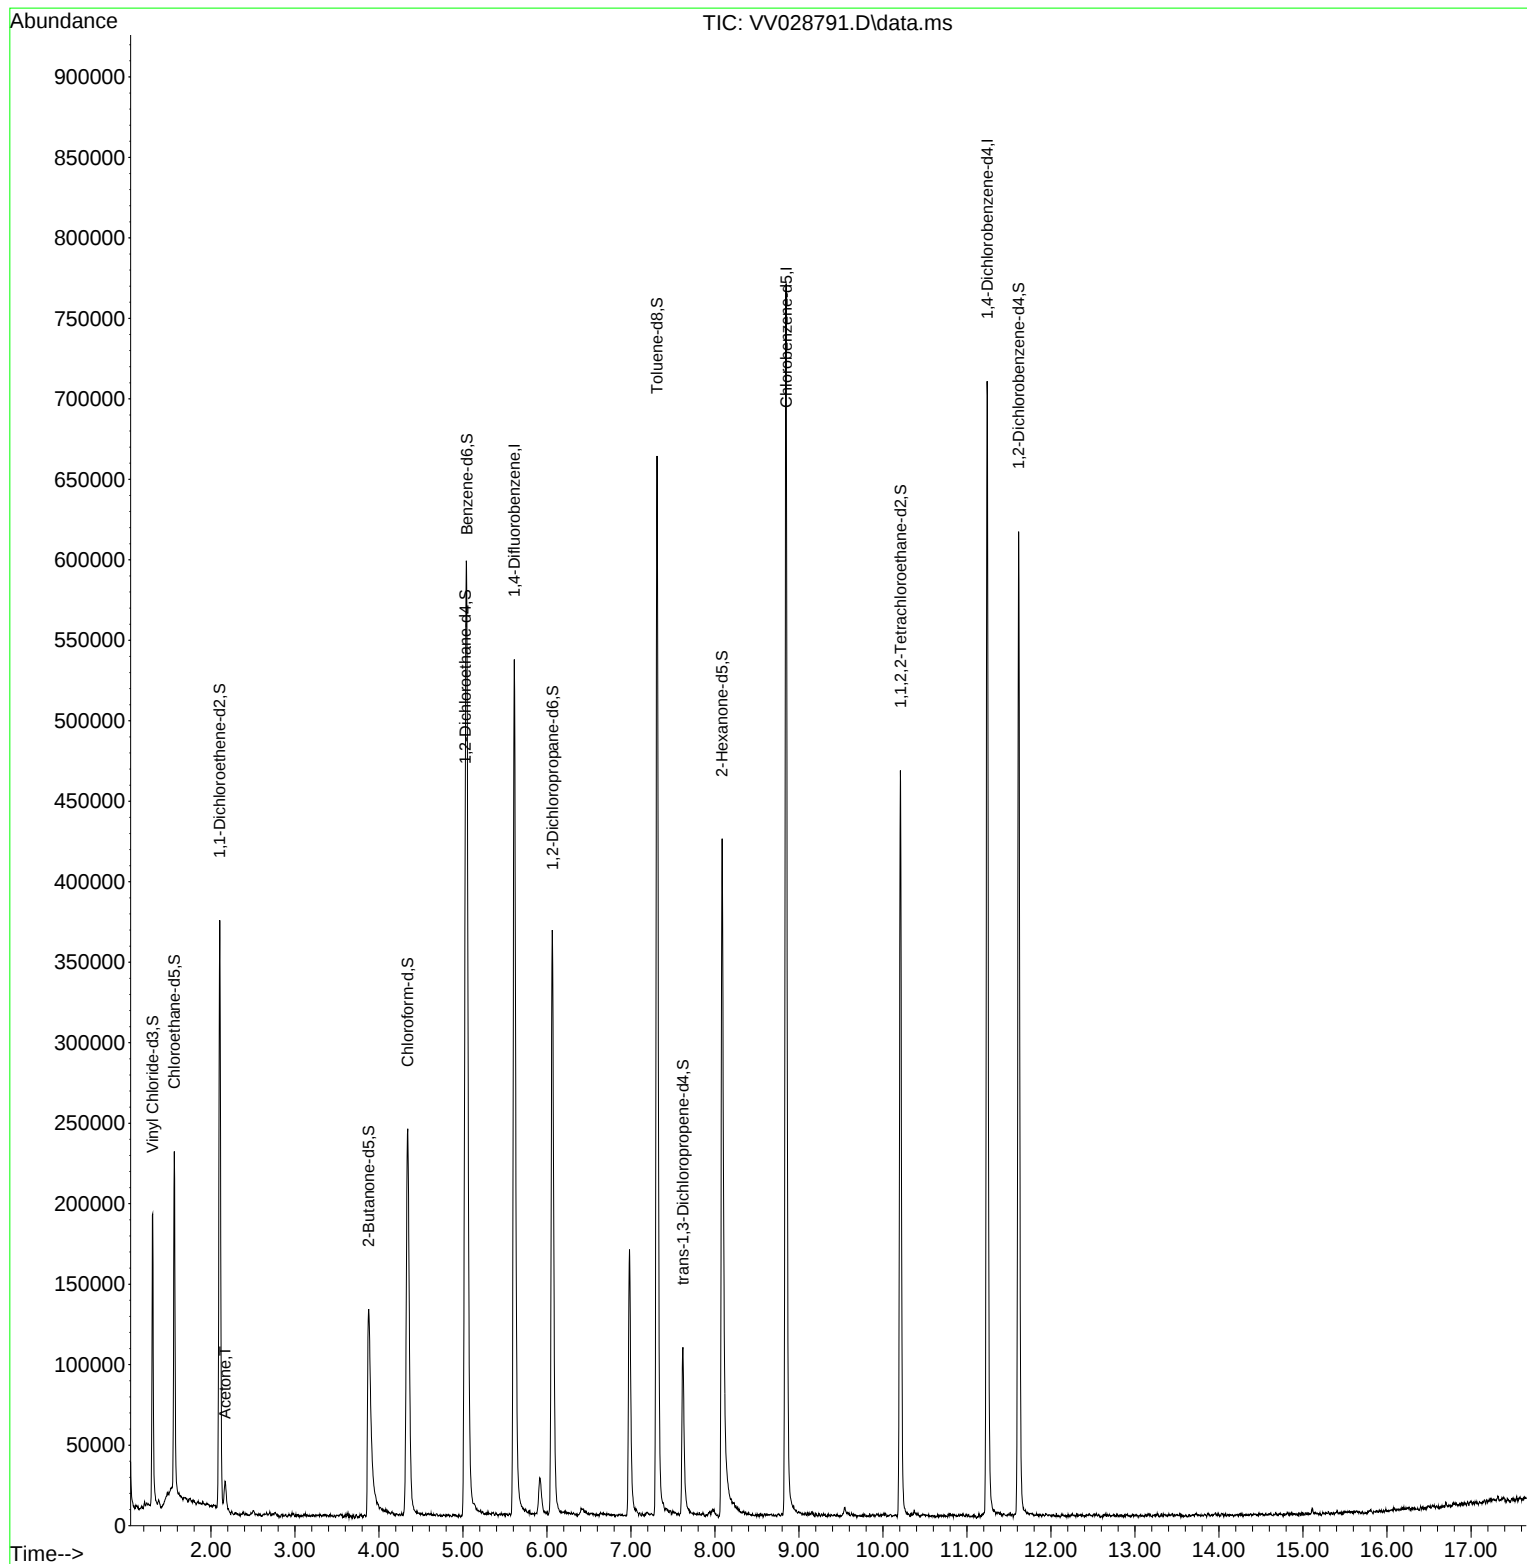

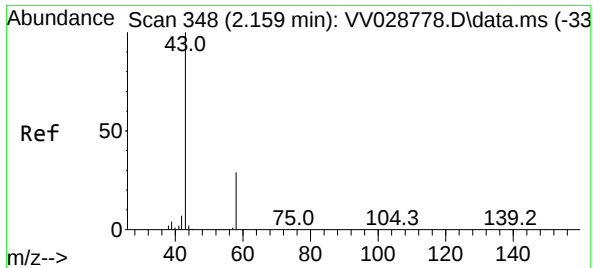

#13
 Acetone
 Concen: 7.698 ug/L
 RT: 2.169 min Scan# 31
 Delta R.T. 0.010 min
 Lab File: VV028791.D
 Acq: 31 Oct 2022 19:31

Instrument :
 MSVOA_V
 ClientSampleId :
 YBMQ0

Tgt Ion: 43 Resp: 22033
 Ion Ratio Lower Upper
 43 100
 58 31.9 0.0 59.0

