

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028783.D
 Acq On : 31 Oct 2022 16:18
 Operator : SY/MD
 Sample : N5301-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWX6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028783.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	96	rVB	199490	211976	6.03%	1.076%
2	1.564	158	163	176	rVB	222674	251849	7.16%	1.279%
3	2.108	323	332	345	rVB	389474	570847	16.23%	2.898%
4	2.503	448	455	461	rBV9	4699	7858	0.22%	0.040%
5	2.635	495	496	498	rBV2	1431	501	0.01%	0.003%
6	2.757	523	534	550	rBV	248541	436157	12.40%	2.214%
7	3.095	635	639	642	rVB4	1858	1520	0.04%	0.008%
8	3.117	643	646	647	rBV3	1105	598	0.02%	0.003%
9	3.275	693	695	702	rBV8	1274	1287	0.04%	0.007%
10	3.301	702	703	705	rBV2	851	385	0.01%	0.002%
11	3.317	705	708	710	rBV4	1730	1016	0.03%	0.005%
12	3.436	742	745	749	rVB6	1296	968	0.03%	0.005%
13	3.474	749	757	758	rBV9	1548	1556	0.04%	0.008%
14	3.516	768	770	772	rBV4	900	404	0.01%	0.002%
15	3.529	772	774	775	rBV2	850	381	0.01%	0.002%
16	3.552	779	781	783	rBV3	881	513	0.01%	0.003%
17	3.593	790	794	796	rBV5	980	814	0.02%	0.004%
18	3.664	810	816	818	rBV6	2083	2414	0.07%	0.012%
19	3.735	835	838	840	rBV4	884	629	0.02%	0.003%
20	3.770	847	849	852	rVB4	1574	1051	0.03%	0.005%
21	3.905	873	891	935	rVV2	1331871	3517158	100.00%	17.855%
22	4.342	1015	1027	1052	rVB	249230	611367	17.38%	3.104%
23	4.786	1163	1165	1167	rBV3	1058	583	0.02%	0.003%
24	4.870	1188	1191	1196	rBV6	1858	1894	0.05%	0.010%
25	4.941	1211	1213	1217	rBV4	1476	677	0.02%	0.003%
26	4.982	1220	1226	1228	rBV7	1517	1619	0.05%	0.008%
27	5.043	1228	1245	1279	rBV2	638146	1666417	47.38%	8.459%
28	5.613	1411	1422	1448	rBV	550667	1118192	31.79%	5.676%
29	5.908	1501	1514	1544	rBV	1170637	2288091	65.06%	11.615%
30	6.066	1552	1563	1585	rVB	384664	769944	21.89%	3.909%
31	6.870	1810	1813	1817	rBV7	1699	1202	0.03%	0.006%
32	6.982	1839	1848	1870	rBV	180015	330859	9.41%	1.680%
33	7.310	1939	1950	1972	rBV	714095	1247642	35.47%	6.334%
34	7.574	2028	2032	2035	rBV6	1948	2125	0.06%	0.011%
35	7.619	2037	2046	2064	rVV	113940	208888	5.94%	1.060%
36	7.825	2108	2110	2111	rBV3	1474	612	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028783.D
 Acq On : 31 Oct 2022 16:18
 Operator : SY/MD
 Sample : N5301-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWX6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	7.915	2134	2138	2140	rBV5	1905	1489	0.04%	0.008%
38	7.969	2144	2155	2180	rVB	728778	1210265	34.41%	6.144%
39	8.085	2182	2191	2221	rBV	436654	843147	23.97%	4.280%
40	8.722	2386	2389	2391	rBV4	1367	804	0.02%	0.004%
41	8.847	2417	2428	2453	rBV	799316	1315732	37.41%	6.679%
42	9.783	2717	2719	2720	rBV2	1394	446	0.01%	0.002%
43	9.812	2726	2728	2732	rVB5	2319	1511	0.04%	0.008%
44	9.831	2732	2734	2735	rBV2	1529	610	0.02%	0.003%
45	9.847	2736	2739	2742	rVV4	1496	1200	0.03%	0.006%
46	9.876	2745	2748	2750	rVB4	1619	1077	0.03%	0.005%
47	9.892	2751	2753	2756	rVV3	1313	646	0.02%	0.003%
48	9.947	2769	2770	2772	rBV	1151	408	0.01%	0.002%
49	10.005	2785	2788	2790	rBV3	1527	1168	0.03%	0.006%
50	10.146	2829	2832	2835	rBV4	1242	1080	0.03%	0.005%
51	10.162	2835	2837	2839	rBV4	1526	887	0.03%	0.005%
52	10.207	2840	2851	2867	rVV	483822	765989	21.78%	3.889%
53	10.365	2896	2900	2902	rBV5	2702	2510	0.07%	0.013%
54	10.535	2950	2953	2954	rBV3	1660	828	0.02%	0.004%
55	10.551	2954	2958	2960	rBV4	2137	1737	0.05%	0.009%
56	10.644	2985	2987	2990	rBV4	1563	1136	0.03%	0.006%
57	10.690	2999	3001	3006	rVB5	1681	1129	0.03%	0.006%
58	10.712	3006	3008	3011	rBV4	1808	1154	0.03%	0.006%
59	10.796	3032	3034	3035	rBV2	1132	460	0.01%	0.002%
60	10.908	3065	3069	3072	rBV6	2814	2522	0.07%	0.013%
61	11.243	3162	3173	3199	rBV	733567	1166082	33.15%	5.920%
62	11.538	3255	3265	3271	rBV	5106	9367	0.27%	0.048%
63	11.616	3278	3289	3315	rVB	664543	1052359	29.92%	5.342%
64	11.815	3350	3351	3352	rBV	1336	485	0.01%	0.002%
65	12.098	3433	3439	3442	rBV8	1806	2181	0.06%	0.011%
66	12.124	3445	3447	3449	rBV2	867	388	0.01%	0.002%
67	12.197	3468	3470	3473	rVB3	2630	1033	0.03%	0.005%
68	12.210	3473	3474	3476	rBV2	1301	629	0.02%	0.003%
69	12.249	3484	3486	3488	rBV3	1484	592	0.02%	0.003%
70	12.300	3496	3502	3504	rBV7	2704	2276	0.06%	0.012%
71	12.326	3507	3510	3512	rBV3	1574	829	0.02%	0.004%
72	12.410	3533	3536	3538	rBV4	1742	1228	0.03%	0.006%
73	12.480	3556	3558	3563	rVB5	1173	744	0.02%	0.004%
74	12.506	3563	3566	3568	rBV4	1191	658	0.02%	0.003%
75	12.519	3568	3570	3574	rBV5	961	665	0.02%	0.003%
76	12.561	3580	3583	3584	rBV3	1163	657	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028783.D
 Acq On : 31 Oct 2022 16:18
 Operator : SY/MD
 Sample : N5301-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWX6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	12.603	3593	3596	3599	rBV5	1783	1294	0.04%	0.007%
78	12.722	3631	3633	3635	rBV3	1197	570	0.02%	0.003%
79	12.812	3658	3661	3663	rBV4	2571	1431	0.04%	0.007%
80	12.847	3670	3672	3674	rBV3	1268	562	0.02%	0.003%
81	12.966	3707	3709	3712	rVB4	1760	857	0.02%	0.004%
82	12.982	3712	3714	3717	rBV3	951	625	0.02%	0.003%
83	13.005	3717	3721	3723	rBV5	1508	897	0.03%	0.005%
84	13.162	3768	3770	3772	rVB3	1784	813	0.02%	0.004%
85	13.236	3789	3793	3795	rBV4	1223	981	0.03%	0.005%
86	13.397	3839	3843	3848	rBV6	1689	1743	0.05%	0.009%
87	13.426	3848	3852	3856	rBV6	1353	1355	0.04%	0.007%
88	13.461	3860	3863	3864	rBV3	1036	659	0.02%	0.003%
89	13.648	3915	3921	3923	rBV5	1391	1317	0.04%	0.007%
90	13.834	3977	3979	3982	rBV4	1428	981	0.03%	0.005%
91	13.934	4007	4010	4011	rBV3	1220	657	0.02%	0.003%
92	13.982	4021	4025	4034	rBV	21933	17430	0.50%	0.088%
93	14.088	4053	4058	4060	rBV5	1549	1539	0.04%	0.008%
94	14.146	4074	4076	4078	rBV3	1418	686	0.02%	0.003%
95	14.300	4122	4124	4125	rBV2	1132	428	0.01%	0.002%
96	14.403	4152	4156	4157	rBV3	1336	968	0.03%	0.005%
97	14.603	4214	4218	4219	rBV4	1508	988	0.03%	0.005%
98	14.705	4246	4250	4252	rBV4	3058	2287	0.07%	0.012%
99	14.757	4262	4266	4267	rBV3	1492	1018	0.03%	0.005%
100	15.056	4357	4359	4361	rBV3	1369	586	0.02%	0.003%




Sum of corrected areas: 19698774

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028783.D
Acq On : 31 Oct 2022 16:18
Operator : SY/MD
Sample : N5301-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWX6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

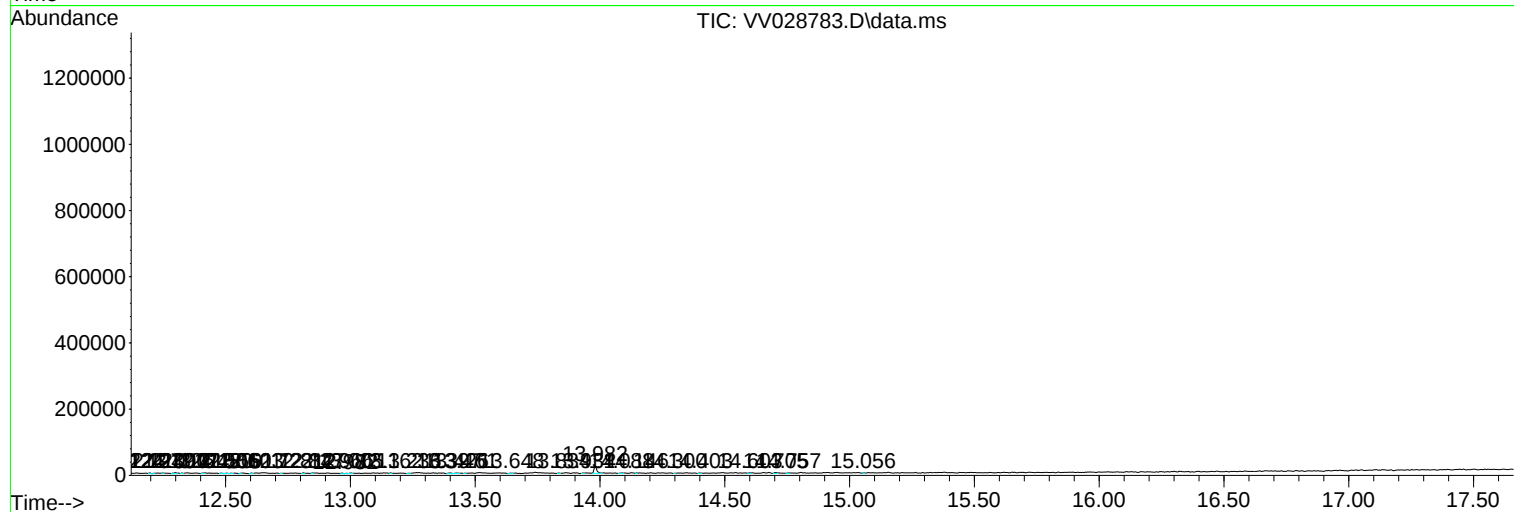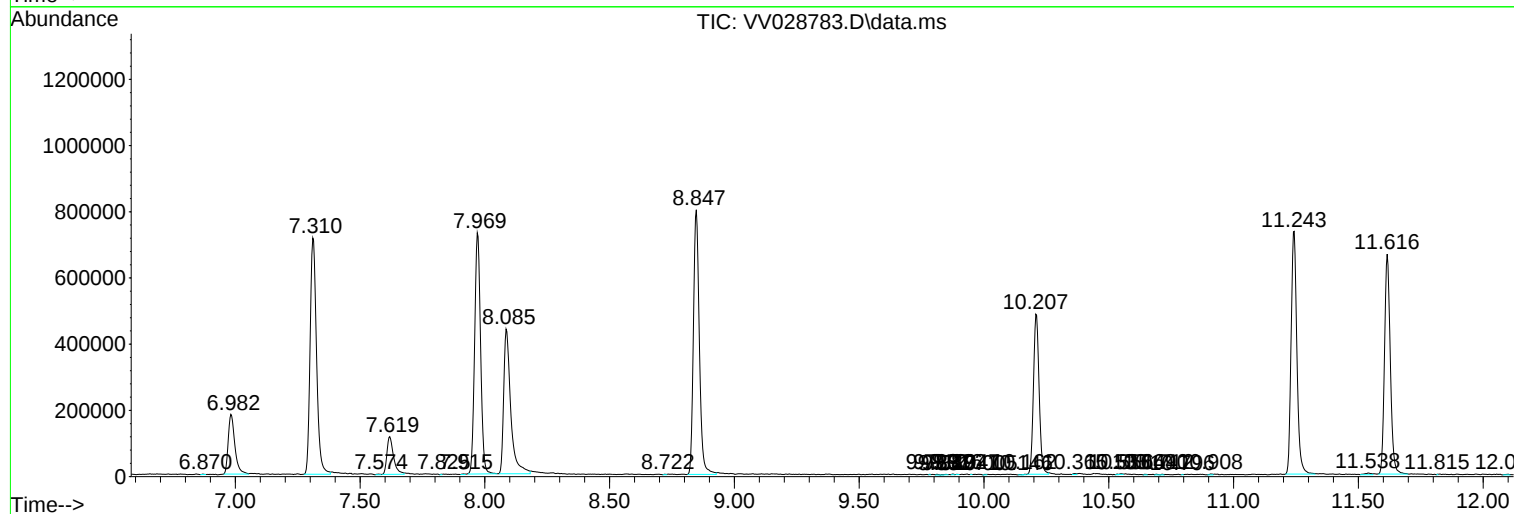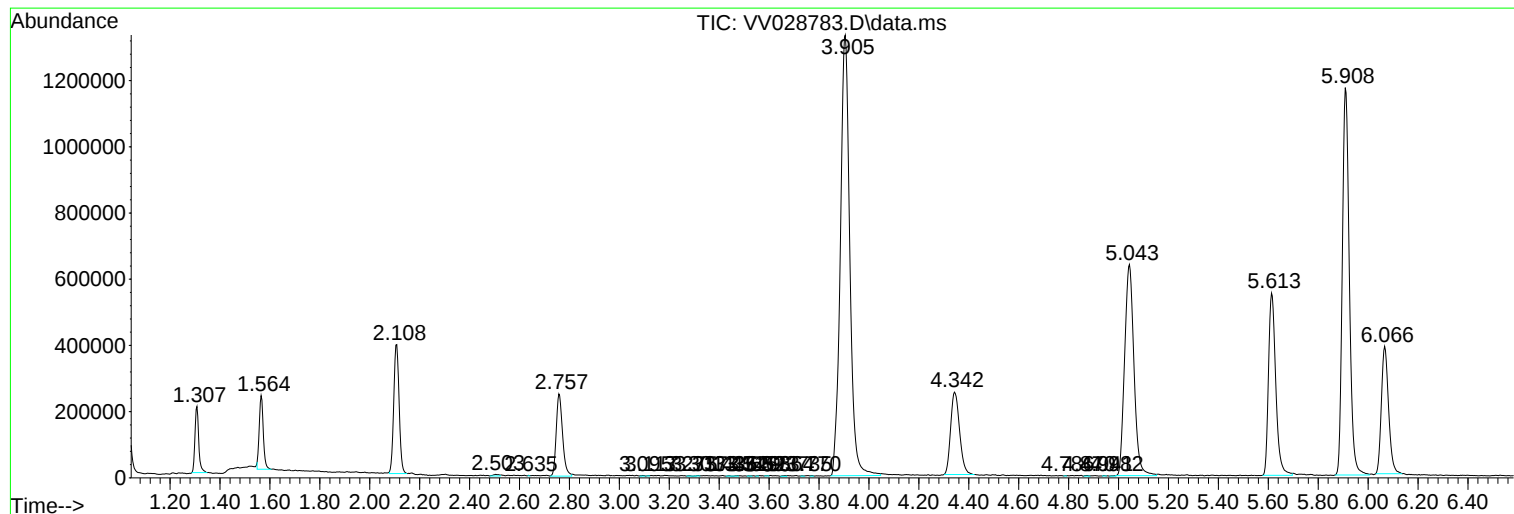

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028783.D
Acq On : 31 Oct 2022 16:18
Operator : SY/MD
Sample : N5301-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWX6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028783.D
Acq On : 31 Oct 2022 16:18
Operator : SY/MD
Sample : N5301-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWX6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc