

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028784.D
 Acq On : 31 Oct 2022 16:42
 Operator : SY/MD
 Sample : N5301-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBXA8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028784.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rBV	243212	259475	3.23%	1.110%
2	1.564	157	163	176	rVB	250088	276182	3.44%	1.181%
3	2.105	322	331	344	rVB	439535	634546	7.91%	2.714%
4	2.757	524	534	556	rVB	338095	582944	7.26%	2.494%
5	3.066	629	630	635	rVB5	1437	779	0.01%	0.003%
6	3.092	636	638	639	rBV2	1087	363	0.00%	0.002%
7	3.307	701	705	710	rBV8	1807	1998	0.02%	0.009%
8	3.397	730	733	736	rVB5	1232	760	0.01%	0.003%
9	3.555	780	782	783	rBV2	1090	338	0.00%	0.001%
10	3.600	793	796	800	rBV5	1710	1465	0.02%	0.006%
11	3.632	804	806	812	rVB7	1435	1122	0.01%	0.005%
12	3.680	817	821	822	rBV4	1110	646	0.01%	0.003%
13	3.725	833	835	837	rVB3	1248	499	0.01%	0.002%
14	3.741	838	840	841	rBV2	1151	381	0.00%	0.002%
15	3.834	867	869	871	rBV2	1092	457	0.01%	0.002%
16	3.902	871	890	928	rBV	3242282	8025552	100.00%	34.332%
17	4.342	1013	1027	1053	rBV	280434	692040	8.62%	2.960%
18	4.513	1077	1080	1083	rBV4	2611	2205	0.03%	0.009%
19	5.040	1228	1244	1283	rBV2	699108	1867697	23.27%	7.990%
20	5.613	1410	1422	1452	rBV	603895	1208930	15.06%	5.172%
21	5.908	1502	1514	1544	rBV	604718	1198359	14.93%	5.126%
22	6.066	1551	1563	1588	rVB	423091	861228	10.73%	3.684%
23	6.342	1646	1649	1652	rBV5	1850	1308	0.02%	0.006%
24	6.635	1736	1740	1742	rBV5	2865	1984	0.02%	0.008%
25	6.847	1804	1806	1810	rVB5	1521	826	0.01%	0.004%
26	6.866	1810	1812	1814	rBV3	812	219	0.00%	0.001%
27	6.879	1814	1816	1817	rBV2	1270	550	0.01%	0.002%
28	6.912	1824	1826	1829	rVB4	1494	726	0.01%	0.003%
29	6.940	1833	1835	1837	rBV3	1369	608	0.01%	0.003%
30	6.982	1838	1848	1864	rBV	204887	367004	4.57%	1.570%
31	7.310	1939	1950	1972	rBV	794029	1371213	17.09%	5.866%
32	7.619	2037	2046	2068	rBV2	129155	227377	2.83%	0.973%
33	8.085	2181	2191	2225	rBV	516859	1013522	12.63%	4.336%
34	8.757	2399	2400	2402	rBV2	1551	507	0.01%	0.002%
35	8.805	2411	2415	2416	rBV3	1683	1116	0.01%	0.005%
36	8.847	2417	2428	2456	rVV	861698	1430123	17.82%	6.118%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028784.D
 Acq On : 31 Oct 2022 16:42
 Operator : SY/MD
 Sample : N5301-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBXA8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	9.239	2549	2550	2552	rBV	1231	505	0.01%	0.002%
38	9.394	2590	2598	2604	rBV	2232	4061	0.05%	0.017%
39	9.439	2604	2612	2615	rBV10	1900	2764	0.03%	0.012%
40	9.484	2624	2626	2628	rBV3	1374	500	0.01%	0.002%
41	9.638	2672	2674	2678	rBV5	1490	882	0.01%	0.004%
42	9.854	2739	2741	2742	rVB2	672	192	0.00%	0.001%
43	9.934	2761	2766	2768	rBV5	1990	1799	0.02%	0.008%
44	10.050	2801	2802	2804	rBV2	1108	395	0.00%	0.002%
45	10.207	2836	2851	2866	rBV	541858	856236	10.67%	3.663%
46	10.490	2936	2939	2942	rBV3	2240	1705	0.02%	0.007%
47	10.526	2948	2950	2952	rBV3	1319	466	0.01%	0.002%
48	10.635	2982	2984	2988	rBV4	761	378	0.00%	0.002%
49	10.661	2989	2992	2994	rBV3	966	638	0.01%	0.003%
50	10.738	3014	3016	3018	rBV3	838	255	0.00%	0.001%
51	10.760	3021	3023	3026	rVV4	1202	694	0.01%	0.003%
52	10.821	3040	3042	3044	rBV3	1478	794	0.01%	0.003%
53	10.850	3050	3051	3054	rBV3	1171	510	0.01%	0.002%
54	10.972	3087	3089	3091	rBV3	929	504	0.01%	0.002%
55	11.005	3097	3099	3101	rVB2	1139	511	0.01%	0.002%
56	11.034	3101	3108	3111	rBV6	2166	2270	0.03%	0.010%
57	11.059	3114	3116	3119	rBV4	1482	973	0.01%	0.004%
58	11.075	3119	3121	3124	rBV4	1196	607	0.01%	0.003%
59	11.146	3142	3143	3144	rBV2	732	200	0.00%	0.001%
60	11.239	3161	3172	3194	rBV	798563	1271774	15.85%	5.440%
61	11.455	3237	3239	3242	rBV3	1349	828	0.01%	0.004%
62	11.471	3242	3244	3245	rBV2	1427	743	0.01%	0.003%
63	11.615	3278	3289	3309	rBV	724320	1155745	14.40%	4.944%
64	11.857	3359	3364	3365	rBV5	1783	1339	0.02%	0.006%
65	11.905	3377	3379	3382	rBV4	1244	855	0.01%	0.004%
66	11.972	3398	3400	3402	rBV3	985	382	0.00%	0.002%
67	12.091	3434	3437	3439	rBV4	2496	1749	0.02%	0.007%
68	12.114	3442	3444	3445	rBV2	1217	439	0.01%	0.002%
69	12.156	3455	3457	3459	rBV3	1266	827	0.01%	0.004%
70	12.197	3469	3470	3471	rBV	926	249	0.00%	0.001%
71	12.271	3491	3493	3496	rVB4	1421	743	0.01%	0.003%
72	12.287	3496	3498	3500	rBV3	1860	1074	0.01%	0.005%
73	12.345	3514	3516	3517	rBV2	932	307	0.00%	0.001%
74	12.445	3546	3547	3549	rBV2	1249	465	0.01%	0.002%
75	12.477	3555	3557	3563	rVB6	1525	1306	0.02%	0.006%
76	12.513	3563	3568	3572	rBV7	2630	2481	0.03%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028784.D
 Acq On : 31 Oct 2022 16:42
 Operator : SY/MD
 Sample : N5301-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBXA8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	12.577	3586	3588	3592	rBV5	1535	782	0.01%	0.003%
78	12.625	3600	3603	3604	rBV3	1006	592	0.01%	0.003%
79	12.635	3604	3606	3607	rBV2	1663	626	0.01%	0.003%
80	12.712	3628	3630	3634	rBV4	1759	1315	0.02%	0.006%
81	12.869	3677	3679	3680	rBV2	1240	461	0.01%	0.002%
82	12.950	3702	3704	3705	rBV	875	337	0.00%	0.001%
83	12.959	3705	3707	3708	rBV2	960	323	0.00%	0.001%
84	13.021	3725	3726	3728	rBV2	988	478	0.01%	0.002%
85	13.162	3769	3770	3771	rBV	941	286	0.00%	0.001%
86	13.191	3777	3779	3782	rBV3	875	396	0.00%	0.002%
87	13.262	3793	3801	3803	rBV9	3622	5137	0.06%	0.022%
88	13.300	3811	3813	3814	rBV2	630	219	0.00%	0.001%
89	13.345	3826	3827	3829	rBV3	1334	557	0.01%	0.002%
90	13.374	3834	3836	3837	rBV2	1027	441	0.01%	0.002%
91	13.670	3927	3928	3929	rBV	1068	251	0.00%	0.001%
92	13.712	3939	3941	3942	rBV2	1310	502	0.01%	0.002%
93	13.802	3968	3969	3972	rVB3	1243	620	0.01%	0.003%
94	13.869	3987	3990	3992	rBV4	2556	1809	0.02%	0.008%
95	13.905	3999	4001	4004	rBV3	1571	963	0.01%	0.004%
96	14.210	4092	4096	4099	rBV6	1567	1349	0.02%	0.006%
97	14.339	4134	4136	4139	rBV3	1180	586	0.01%	0.003%
98	14.873	4299	4302	4307	rBV6	2338	2483	0.03%	0.011%
99	15.345	4447	4449	4452	rBV3	1914	1021	0.01%	0.004%
100	15.538	4508	4509	4510	rBV	1764	631	0.01%	0.003%




Sum of corrected areas: 23376359

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028784.D
Acq On : 31 Oct 2022 16:42
Operator : SY/MD
Sample : N5301-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBXA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

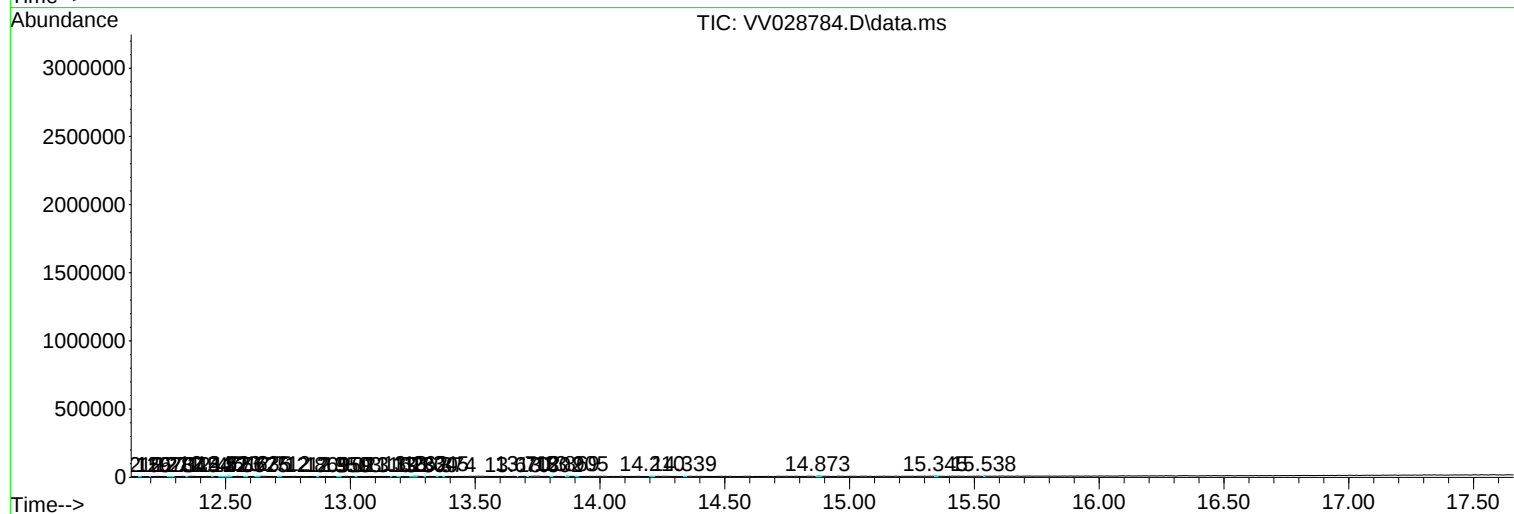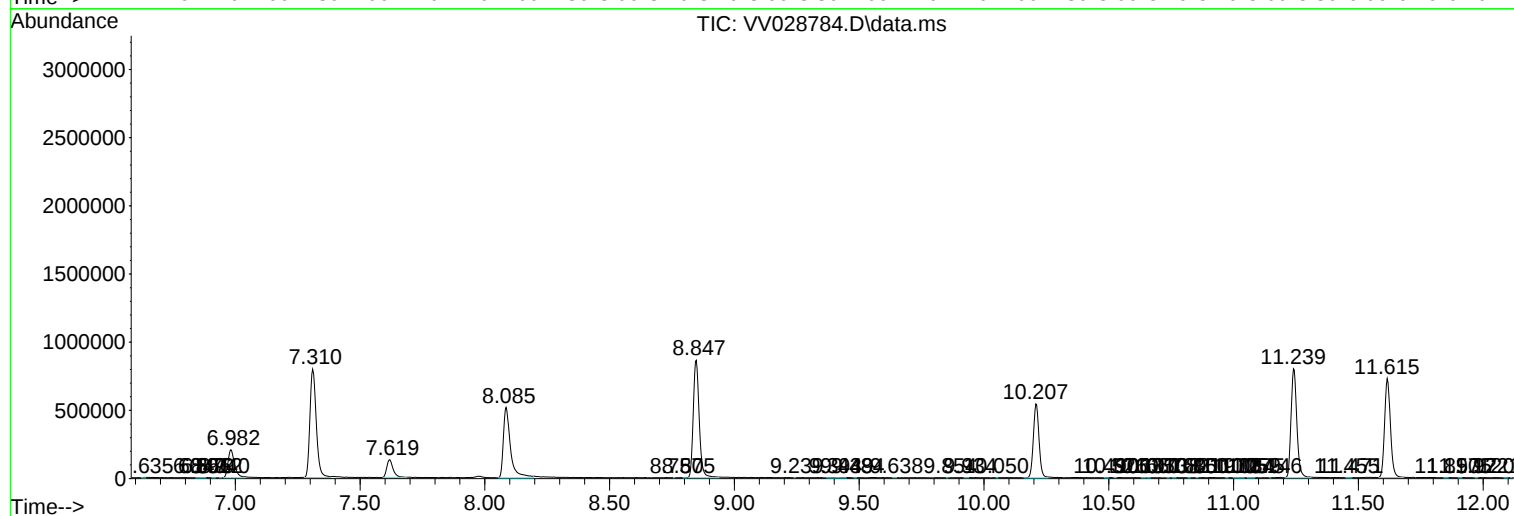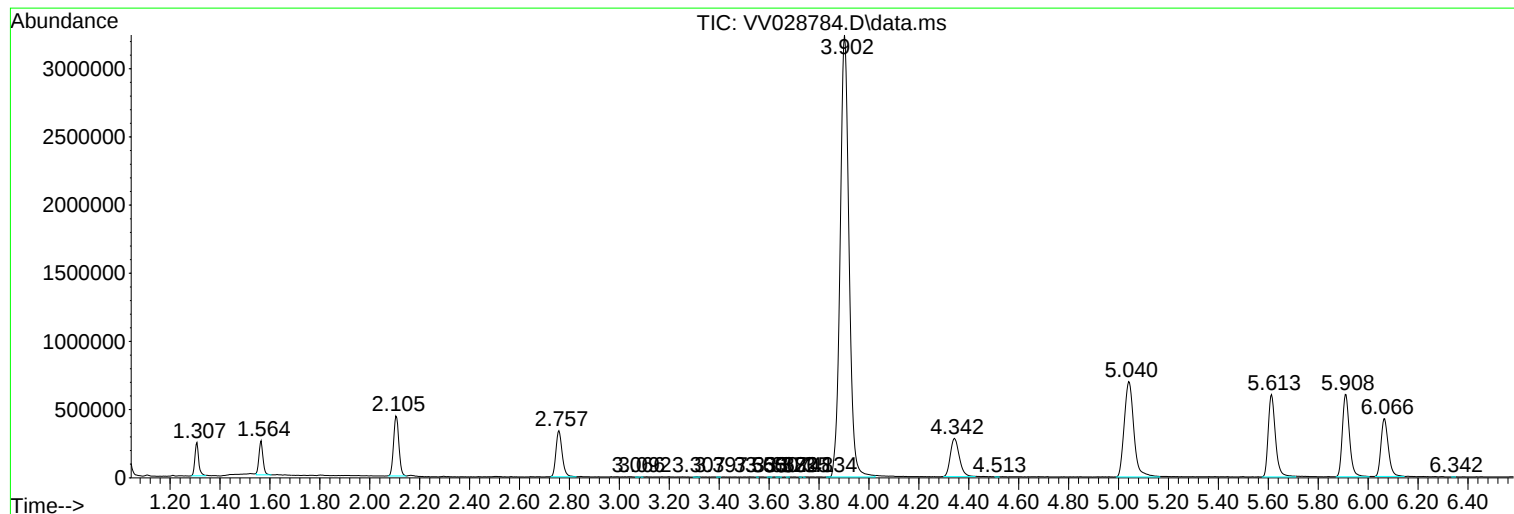

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028784.D
Acq On : 31 Oct 2022 16:42
Operator : SY/MD
Sample : N5301-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBXA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028784.D
Acq On : 31 Oct 2022 16:42
Operator : SY/MD
Sample : N5301-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBXA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc