

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028786.D
 Acq On : 31 Oct 2022 17:30
 Operator : SY/MD
 Sample : N5354-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBMP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028786.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	101	rVB	191748	212792	13.06%	1.678%
2	1.565	157	163	177	rVB	223304	256013	15.72%	2.019%
3	2.105	323	331	343	rVB	384181	544765	33.44%	4.297%
4	2.555	469	471	475	rVB5	1447	841	0.05%	0.007%
5	2.799	544	547	551	rBV6	1517	1441	0.09%	0.011%
6	2.931	586	588	589	rBV2	1276	488	0.03%	0.004%
7	3.040	620	622	627	rVB6	1738	981	0.06%	0.008%
8	3.175	659	664	666	rBV6	2160	1749	0.11%	0.014%
9	3.282	696	697	699	rVB2	1516	504	0.03%	0.004%
10	3.323	708	710	712	rBV3	1053	545	0.03%	0.004%
11	3.465	752	754	756	rVB2	1506	599	0.04%	0.005%
12	3.561	778	784	787	rBV7	1251	1275	0.08%	0.010%
13	3.619	800	802	804	rVB3	1719	777	0.05%	0.006%
14	3.642	804	809	810	rBV5	2109	1903	0.12%	0.015%
15	3.700	823	827	832	rBV6	1671	1444	0.09%	0.011%
16	3.741	838	840	843	rBV4	1564	802	0.05%	0.006%
17	3.809	857	861	864	rBV5	1024	978	0.06%	0.008%
18	3.876	873	882	913	rBV	136455	401648	24.66%	3.168%
19	4.343	1013	1027	1050	rBV	248581	614612	37.73%	4.848%
20	4.542	1087	1089	1091	rBV3	1450	662	0.04%	0.005%
21	4.732	1146	1148	1150	rBV3	1497	709	0.04%	0.006%
22	4.754	1153	1155	1157	rVB3	1434	558	0.03%	0.004%
23	4.809	1170	1172	1174	rBV3	1449	776	0.05%	0.006%
24	4.841	1180	1182	1184	rBV3	1319	590	0.04%	0.005%
25	4.889	1190	1197	1199	rBV7	1520	2123	0.13%	0.017%
26	4.941	1211	1213	1215	rBV3	1614	992	0.06%	0.008%
27	5.040	1228	1244	1267	rBV2	625805	1628970	100.00%	12.849%
28	5.317	1328	1330	1333	rBV4	1663	1223	0.08%	0.010%
29	5.613	1410	1422	1448	rVV	561774	1133310	69.57%	8.939%
30	6.066	1551	1563	1586	rBV	381092	771648	47.37%	6.087%
31	6.410	1665	1670	1674	rBV8	2178	2418	0.15%	0.019%
32	6.532	1706	1708	1711	rVB4	1542	694	0.04%	0.005%
33	6.564	1716	1718	1720	rBV3	1898	746	0.05%	0.006%
34	6.625	1733	1737	1740	rBV5	3053	2641	0.16%	0.021%
35	6.851	1803	1807	1810	rVB6	2353	2007	0.12%	0.016%
36	6.867	1810	1812	1813	rBV2	1188	589	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028786.D
 Acq On : 31 Oct 2022 17:30
 Operator : SY/MD
 Sample : N5354-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBMP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	6.915	1825	1827	1829	rBV3	1771	1108	0.07%	0.009%
38	6.982	1838	1848	1864	rBV	177624	318732	19.57%	2.514%
39	7.310	1936	1950	1972	rBV	710256	1236969	75.94%	9.757%
40	7.619	2037	2046	2064	rBV	111397	203474	12.49%	1.605%
41	7.973	2148	2156	2167	rVB3	32637	53797	3.30%	0.424%
42	8.085	2182	2191	2221	rBV	443832	878576	53.93%	6.930%
43	8.738	2389	2394	2399	rBV8	1854	2238	0.14%	0.018%
44	8.767	2399	2403	2405	rBV4	1135	849	0.05%	0.007%
45	8.847	2417	2428	2452	rBV	810268	1341056	82.33%	10.578%
46	9.352	2583	2585	2587	rBV3	1393	679	0.04%	0.005%
47	9.400	2596	2600	2602	rBV4	1041	862	0.05%	0.007%
48	9.545	2638	2645	2658	rVB	11789	18076	1.11%	0.143%
49	9.770	2711	2715	2720	rVB7	2139	1915	0.12%	0.015%
50	9.793	2720	2722	2726	rBV4	1875	1599	0.10%	0.013%
51	9.847	2733	2739	2742	rBV8	1443	1205	0.07%	0.010%
52	9.863	2742	2744	2747	rBV4	1509	775	0.05%	0.006%
53	9.918	2758	2761	2764	rBV4	2287	1476	0.09%	0.012%
54	9.976	2775	2779	2781	rBV4	2584	1966	0.12%	0.016%
55	10.047	2799	2801	2802	rBV2	1536	691	0.04%	0.005%
56	10.207	2840	2851	2870	rBV	490304	773855	47.51%	6.104%
57	10.413	2913	2915	2917	rBV3	922	517	0.03%	0.004%
58	10.455	2926	2928	2929	rBV2	1300	488	0.03%	0.004%
59	10.513	2943	2946	2947	rBV3	1060	604	0.04%	0.005%
60	10.587	2967	2969	2973	rVB5	1740	1013	0.06%	0.008%
61	10.606	2973	2975	2979	rBV5	1487	1052	0.06%	0.008%
62	10.674	2994	2996	2999	rBV3	952	699	0.04%	0.006%
63	10.706	3001	3006	3011	rBV8	1949	1998	0.12%	0.016%
64	10.841	3045	3048	3049	rBV3	1244	568	0.03%	0.004%
65	10.854	3049	3052	3053	rBV3	1495	602	0.04%	0.005%
66	11.149	3142	3144	3146	rBV3	1214	545	0.03%	0.004%
67	11.162	3146	3148	3150	rBV3	1282	733	0.04%	0.006%
68	11.239	3160	3172	3198	rBV	753196	1188870	72.98%	9.378%
69	11.616	3278	3289	3306	rBV	639812	1013222	62.20%	7.992%
70	11.792	3342	3344	3345	rBV2	1385	570	0.03%	0.004%
71	11.998	3404	3408	3409	rBV4	2165	1245	0.08%	0.010%
72	12.046	3420	3423	3425	rBV4	1657	1014	0.06%	0.008%
73	12.188	3464	3467	3469	rBV4	809	552	0.03%	0.004%
74	12.255	3484	3488	3490	rBV5	1959	1417	0.09%	0.011%
75	12.284	3495	3497	3499	rBV3	1644	953	0.06%	0.008%
76	12.345	3514	3516	3520	rBV4	1121	802	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028786.D
 Acq On : 31 Oct 2022 17:30
 Operator : SY/MD
 Sample : N5354-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBMP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	12.484	3555	3559	3560	rBV3	1819	1022	0.06%	0.008%
78	12.645	3605	3609	3611	rBV5	2907	1983	0.12%	0.016%
79	12.690	3621	3623	3625	rBV3	1457	758	0.05%	0.006%
80	12.770	3646	3648	3650	rBV3	1444	827	0.05%	0.007%
81	12.915	3692	3693	3695	rBV2	1139	513	0.03%	0.004%
82	12.927	3695	3697	3698	rVV2	1446	481	0.03%	0.004%
83	12.966	3707	3709	3716	rVB7	1552	1082	0.07%	0.009%
84	13.053	3734	3736	3740	rVB5	1579	995	0.06%	0.008%
85	13.082	3742	3745	3747	rBV5	1610	878	0.05%	0.007%
86	13.178	3773	3775	3776	rBV2	1333	621	0.04%	0.005%
87	13.239	3790	3794	3797	rBV5	1699	1531	0.09%	0.012%
88	13.272	3801	3804	3805	rBV3	1712	819	0.05%	0.006%
89	13.304	3812	3814	3817	rBV3	1243	491	0.03%	0.004%
90	13.500	3869	3875	3880	rBV8	2620	3904	0.24%	0.031%
91	13.664	3923	3926	3929	rBV5	1745	1261	0.08%	0.010%
92	13.693	3933	3935	3936	rBV3	1115	500	0.03%	0.004%
93	13.731	3945	3947	3948	rBV2	1640	585	0.04%	0.005%
94	13.770	3957	3959	3961	rVB3	2446	1150	0.07%	0.009%
95	13.796	3964	3967	3969	rBV4	1720	1108	0.07%	0.009%
96	13.966	4017	4020	4022	rBV4	1455	1019	0.06%	0.008%
97	14.027	4037	4039	4041	rBV3	1415	635	0.04%	0.005%
98	14.226	4098	4101	4102	rBV3	1798	1136	0.07%	0.009%
99	14.493	4182	4184	4186	rBV3	1401	622	0.04%	0.005%
100	14.847	4292	4294	4299	rVB5	2241	1576	0.10%	0.012%




Sum of corrected areas: 12677672

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028786.D
Acq On : 31 Oct 2022 17:30
Operator : SY/MD
Sample : N5354-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBMP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

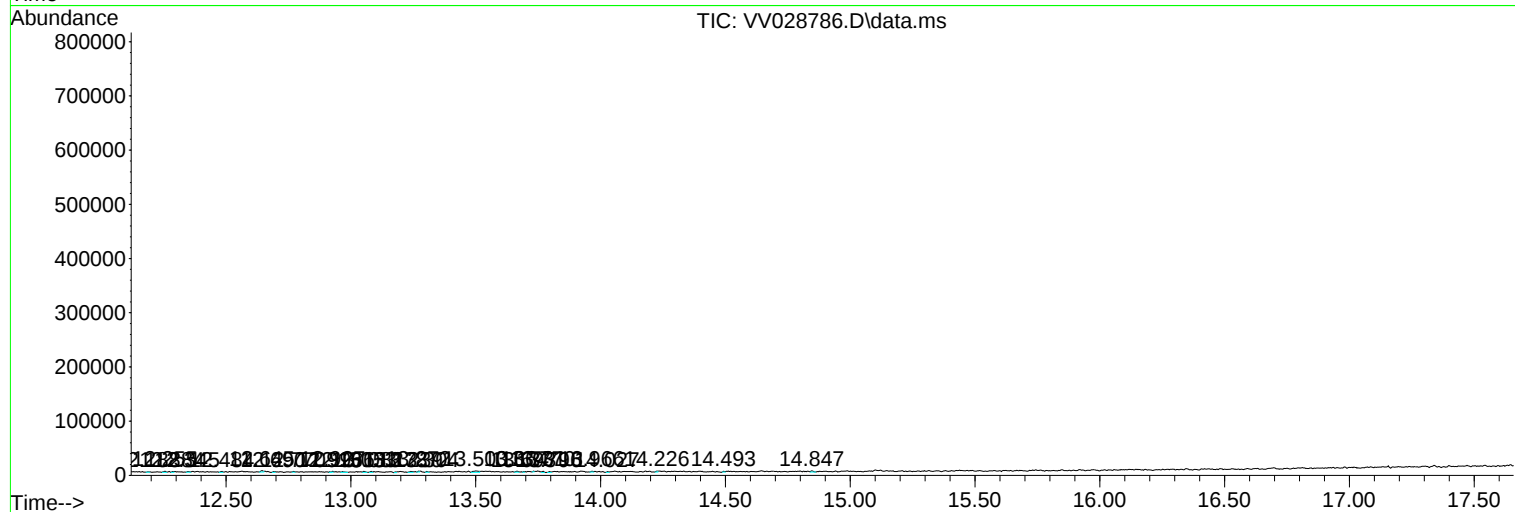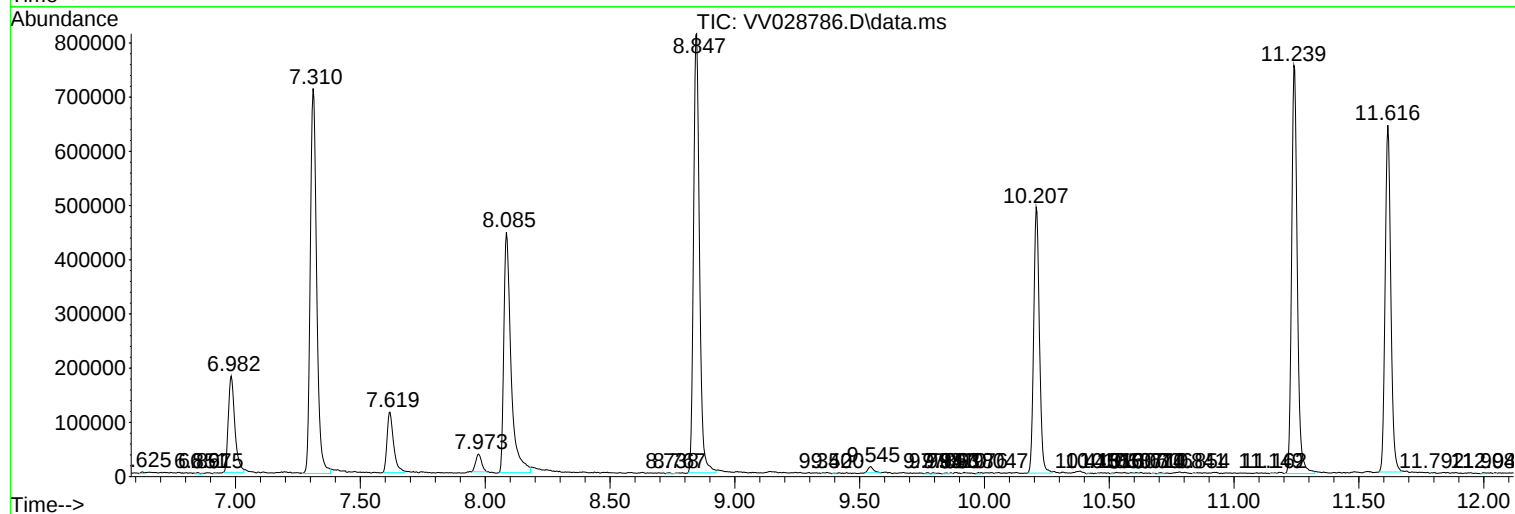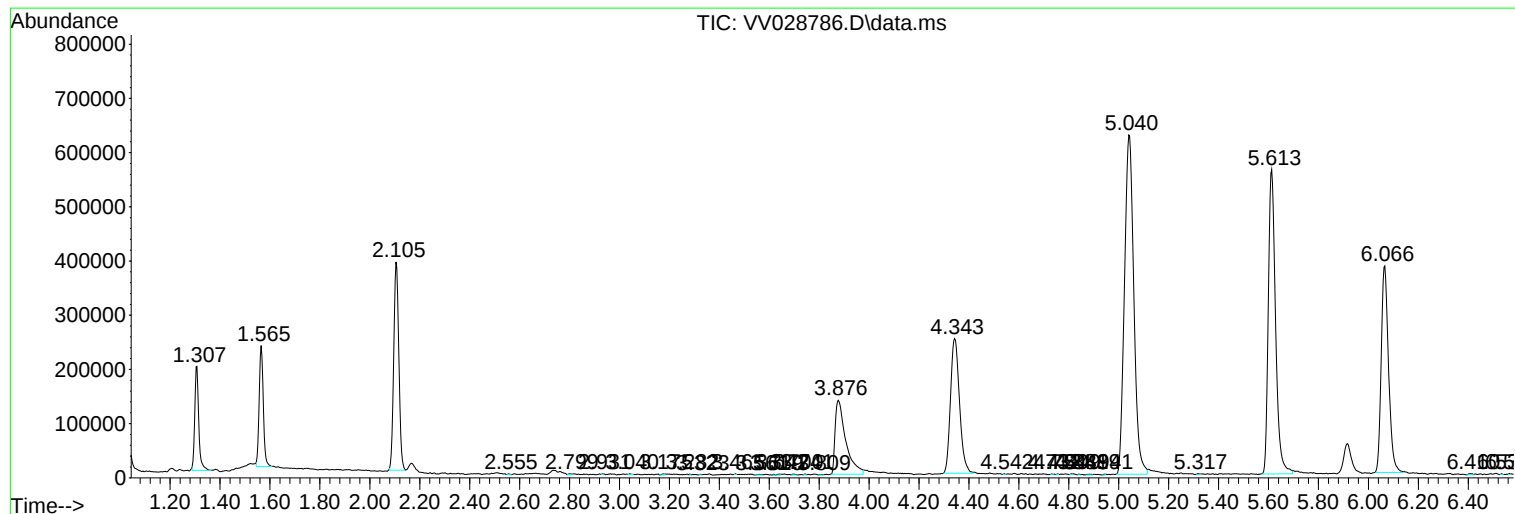

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028786.D
Acq On : 31 Oct 2022 17:30
Operator : SY/MD
Sample : N5354-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBMP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028786.D
Acq On : 31 Oct 2022 17:30
Operator : SY/MD
Sample : N5354-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBMP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc