

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028787.D
 Acq On : 31 Oct 2022 17:54
 Operator : SY/MD
 Sample : N5354-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBMP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028787.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	16	21	31	rBV	34869	33687	2.10%	0.253%
2	1.304	76	82	100	rVB	206187	237052	14.74%	1.780%
3	1.564	157	163	179	rVB	222314	253870	15.79%	1.906%
4	2.104	322	331	342	rBV	381081	548898	34.14%	4.122%
5	2.166	343	350	370	rVB	147222	279288	17.37%	2.097%
6	2.812	549	551	554	rBV4	1220	964	0.06%	0.007%
7	3.011	610	613	615	rBV4	1470	817	0.05%	0.006%
8	3.076	631	633	635	rBV3	1435	901	0.06%	0.007%
9	3.101	640	641	645	rBV4	946	432	0.03%	0.003%
10	3.127	645	649	651	rBV4	1840	1320	0.08%	0.010%
11	3.239	682	684	686	rVB3	1299	511	0.03%	0.004%
12	3.256	687	689	690	rBV2	1142	430	0.03%	0.003%
13	3.346	714	717	718	rBV2	915	448	0.03%	0.003%
14	3.365	721	723	725	rVV3	875	535	0.03%	0.004%
15	3.397	729	733	734	rBV4	1292	876	0.05%	0.007%
16	3.436	741	745	749	rBV7	883	900	0.06%	0.007%
17	3.596	792	795	797	rBV4	1384	1099	0.07%	0.008%
18	3.651	808	812	815	rBV5	1660	1123	0.07%	0.008%
19	3.741	837	840	841	rBV3	748	429	0.03%	0.003%
20	3.767	846	848	850	rVV3	1443	770	0.05%	0.006%
21	3.793	854	856	858	rBV2	932	604	0.04%	0.005%
22	3.876	873	882	909	rBV	131124	381417	23.72%	2.864%
23	4.342	1012	1027	1054	rBV	248017	624931	38.86%	4.693%
24	4.751	1151	1154	1156	rBV4	2426	1331	0.08%	0.010%
25	4.969	1220	1222	1223	rBV2	1187	492	0.03%	0.004%
26	5.043	1228	1245	1269	rVV2	613431	1607958	100.00%	12.075%
27	5.458	1372	1374	1375	rBV2	1315	379	0.02%	0.003%
28	5.503	1387	1388	1390	rBV2	1459	741	0.05%	0.006%
29	5.612	1410	1422	1441	rBV	534993	1082398	67.32%	8.128%
30	5.911	1504	1515	1538	rBV	284210	555128	34.52%	4.169%
31	6.066	1552	1563	1587	rVB	375075	758802	47.19%	5.698%
32	6.223	1609	1612	1614	rBV3	2208	1196	0.07%	0.009%
33	6.378	1658	1660	1663	rBV4	2197	915	0.06%	0.007%
34	6.423	1669	1674	1679	rBV9	2445	3284	0.20%	0.025%
35	6.776	1782	1784	1785	rBV2	1255	543	0.03%	0.004%
36	6.828	1797	1800	1803	rBV4	1538	1278	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028787.D
 Acq On : 31 Oct 2022 17:54
 Operator : SY/MD
 Sample : N5354-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBMP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	6.915	1824	1827	1832	rBV6	1344	1110	0.07%	0.008%
38	6.982	1837	1848	1867	rBV	175033	325781	20.26%	2.446%
39	7.310	1938	1950	1975	rBV	692530	1218559	75.78%	9.151%
40	7.619	2037	2046	2064	rBV	112480	196997	12.25%	1.479%
41	7.972	2149	2156	2168	rVB2	41721	68335	4.25%	0.513%
42	8.085	2181	2191	2224	rBV	434736	876141	54.49%	6.579%
43	8.413	2291	2293	2297	rBV5	2057	1461	0.09%	0.011%
44	8.779	2403	2407	2409	rBV5	2002	1726	0.11%	0.013%
45	8.792	2409	2411	2413	rVV2	1685	703	0.04%	0.005%
46	8.847	2417	2428	2457	rVV	783570	1293317	80.43%	9.712%
47	9.239	2548	2550	2553	rBV4	1323	735	0.05%	0.006%
48	9.403	2599	2601	2607	rBV6	1328	844	0.05%	0.006%
49	9.461	2616	2619	2620	rBV3	2082	1105	0.07%	0.008%
50	9.471	2620	2622	2624	rVV3	1274	606	0.04%	0.005%
51	9.705	2692	2695	2698	rBV5	1343	1117	0.07%	0.008%
52	9.750	2703	2709	2713	rBV9	1718	2156	0.13%	0.016%
53	9.931	2763	2765	2767	rBV3	1201	730	0.05%	0.005%
54	10.017	2789	2792	2793	rBV3	1291	771	0.05%	0.006%
55	10.130	2825	2827	2829	rBV3	1520	747	0.05%	0.006%
56	10.207	2840	2851	2868	rBV	476303	756038	47.02%	5.677%
57	10.345	2891	2894	2897	rBV4	2861	2041	0.13%	0.015%
58	10.429	2914	2920	2923	rBV7	2608	2890	0.18%	0.022%
59	10.467	2930	2932	2934	rBV3	1153	599	0.04%	0.004%
60	10.477	2934	2935	2939	rVB4	2164	912	0.06%	0.007%
61	10.541	2952	2955	2958	rBV5	1555	1277	0.08%	0.010%
62	10.625	2979	2981	2984	rBV4	1025	438	0.03%	0.003%
63	10.770	3024	3026	3031	rVB6	1533	891	0.06%	0.007%
64	10.802	3034	3036	3039	rVB4	1767	938	0.06%	0.007%
65	10.889	3060	3063	3064	rBV3	1730	932	0.06%	0.007%
66	11.021	3102	3104	3107	rBV4	1109	799	0.05%	0.006%
67	11.088	3122	3125	3129	rVB6	1659	1342	0.08%	0.010%
68	11.172	3148	3151	3153	rBV4	1017	626	0.04%	0.005%
69	11.239	3162	3172	3194	rBV	707829	1125793	70.01%	8.454%
70	11.615	3278	3289	3315	rBV	632990	1011853	62.93%	7.599%
71	11.972	3394	3400	3401	rBV5	1838	1801	0.11%	0.014%
72	12.046	3420	3423	3426	rBV5	1176	830	0.05%	0.006%
73	12.120	3442	3446	3447	rBV4	1862	1437	0.09%	0.011%
74	12.162	3455	3459	3461	rBV5	2361	1840	0.11%	0.014%
75	12.307	3500	3504	3506	rBV5	2336	1884	0.12%	0.014%
76	12.493	3560	3562	3565	rVB4	1922	1081	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028787.D
 Acq On : 31 Oct 2022 17:54
 Operator : SY/MD
 Sample : N5354-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBMP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	12.512	3565	3568	3570	rBV4	1646	706	0.04%	0.005%
78	12.535	3570	3575	3577	rBV5	1240	1046	0.07%	0.008%
79	12.586	3588	3591	3592	rBV3	821	488	0.03%	0.004%
80	12.609	3595	3598	3601	rVV5	1928	1343	0.08%	0.010%
81	12.628	3601	3604	3606	rVV4	1700	1075	0.07%	0.008%
82	12.651	3609	3611	3615	rVB4	2085	966	0.06%	0.007%
83	12.670	3615	3617	3619	rBV3	1228	606	0.04%	0.005%
84	12.789	3651	3654	3655	rBV2	1450	876	0.05%	0.007%
85	12.815	3660	3662	3664	rBV3	1283	645	0.04%	0.005%
86	12.885	3682	3684	3689	rVB6	1871	1271	0.08%	0.010%
87	13.040	3730	3732	3734	rBV4	1045	667	0.04%	0.005%
88	13.078	3739	3744	3747	rVV6	1431	1168	0.07%	0.009%
89	13.345	3825	3827	3828	rBV3	1374	496	0.03%	0.004%
90	13.455	3858	3861	3864	rBV4	1593	1061	0.07%	0.008%
91	13.583	3899	3901	3904	rBV4	1247	609	0.04%	0.005%
92	13.631	3913	3916	3918	rBV4	2145	1272	0.08%	0.010%
93	13.728	3944	3946	3948	rBV3	1386	654	0.04%	0.005%
94	13.930	4005	4009	4010	rBV3	1737	1195	0.07%	0.009%
95	13.966	4019	4020	4026	rBV5	1339	1150	0.07%	0.009%
96	14.136	4071	4073	4076	rBV4	1634	908	0.06%	0.007%
97	14.178	4085	4086	4088	rBV2	915	383	0.02%	0.003%
98	14.217	4096	4098	4101	rVB3	1713	801	0.05%	0.006%
99	14.799	4276	4279	4284	rBV7	1435	1457	0.09%	0.011%
100	15.210	4405	4407	4409	rBV3	1491	706	0.04%	0.005%




Sum of corrected areas: 13316479

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028787.D
Acq On : 31 Oct 2022 17:54
Operator : SY/MD
Sample : N5354-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBMP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

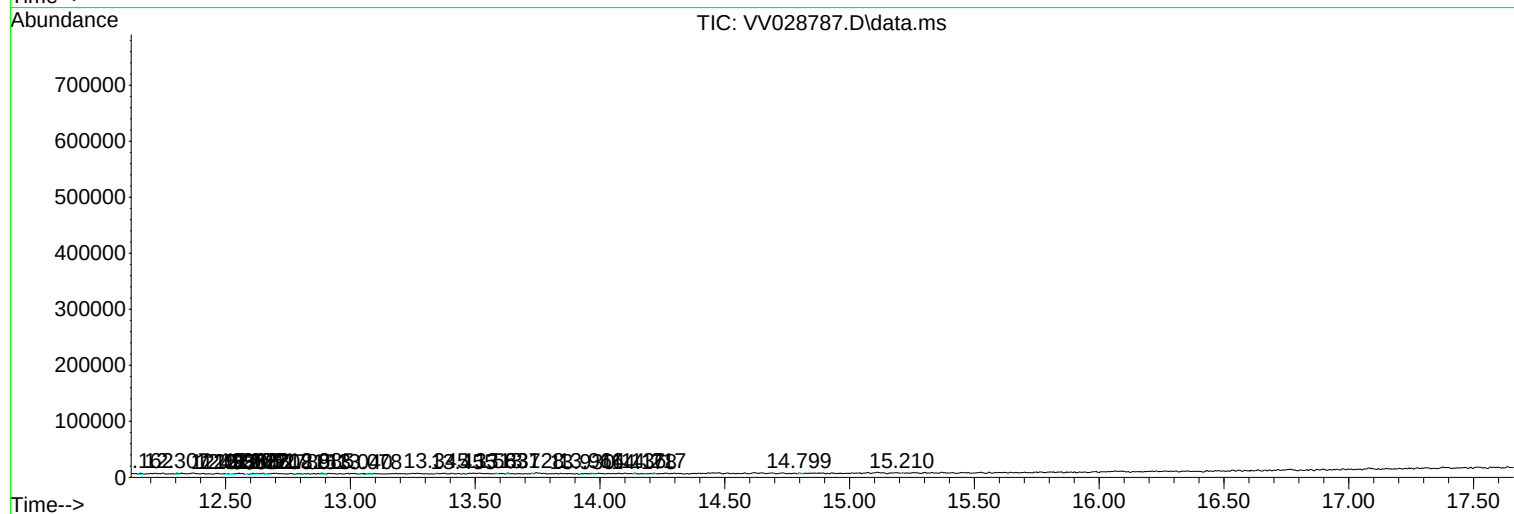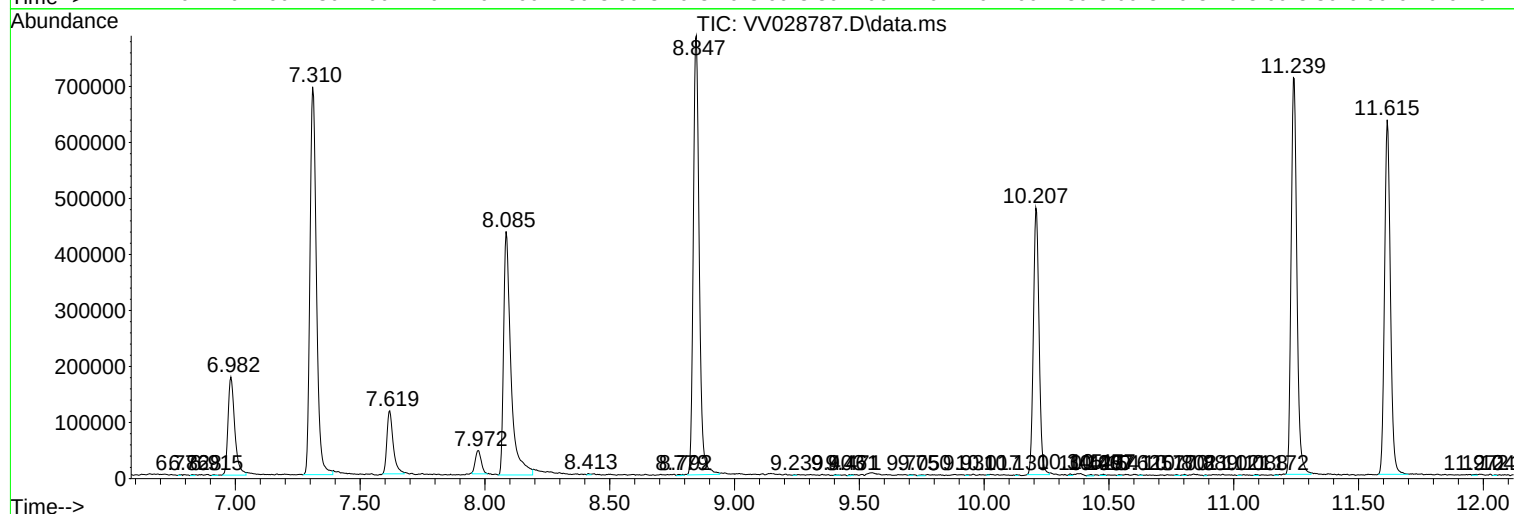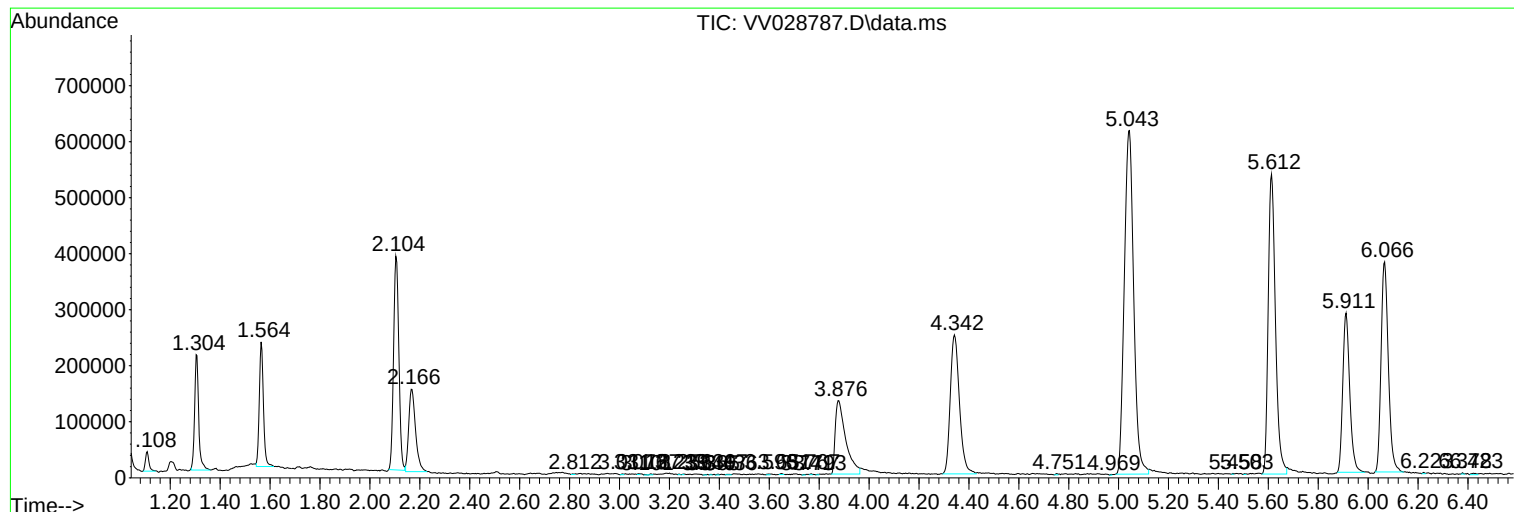

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028787.D
Acq On : 31 Oct 2022 17:54
Operator : SY/MD
Sample : N5354-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBMP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028787.D
Acq On : 31 Oct 2022 17:54
Operator : SY/MD
Sample : N5354-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBMP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc