

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028788.D
 Acq On : 31 Oct 2022 18:18
 Operator : SY/MD
 Sample : N5354-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBMP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028788.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	45	50	58	rBV2	30974	30919	1.96%	0.251%
2	1.307	76	83	102	rVB	182637	204908	13.00%	1.662%
3	1.565	157	163	184	rVB	218085	260282	16.51%	2.111%
4	2.105	322	331	341	rBV	371145	530084	33.62%	4.299%
5	2.166	342	350	368	rVB	178267	312139	19.80%	2.531%
6	2.568	472	475	479	rBV5	2391	1438	0.09%	0.012%
7	2.606	484	487	491	rBV6	2259	2414	0.15%	0.020%
8	3.185	665	667	669	rBV3	1663	851	0.05%	0.007%
9	3.220	674	678	680	rBV3	1602	1129	0.07%	0.009%
10	3.249	684	687	688	rBV3	1164	585	0.04%	0.005%
11	3.262	688	691	694	rVB5	1452	1028	0.07%	0.008%
12	3.281	694	697	698	rBV3	863	484	0.03%	0.004%
13	3.317	706	708	710	rBV3	892	436	0.03%	0.004%
14	3.359	719	721	723	rBV3	1000	373	0.02%	0.003%
15	3.455	750	751	753	rVB2	1867	649	0.04%	0.005%
16	3.465	753	754	756	rVB2	798	274	0.02%	0.002%
17	3.478	756	758	760	rBV3	1729	986	0.06%	0.008%
18	3.571	786	787	789	rBV2	559	154	0.01%	0.001%
19	3.635	806	807	809	rBV2	778	207	0.01%	0.002%
20	3.690	822	824	826	rVB3	1527	406	0.03%	0.003%
21	3.876	873	882	912	rBV	129559	372773	23.65%	3.023%
22	4.343	1014	1027	1049	rVB	240112	579258	36.74%	4.697%
23	4.603	1103	1108	1110	rBV6	1914	1622	0.10%	0.013%
24	4.748	1151	1153	1154	rBV2	1082	441	0.03%	0.004%
25	4.786	1163	1165	1166	rBV2	1863	792	0.05%	0.006%
26	4.876	1192	1193	1196	rBV3	1223	579	0.04%	0.005%
27	4.941	1212	1213	1215	rBV2	1317	644	0.04%	0.005%
28	4.986	1223	1227	1228	rBV3	1715	922	0.06%	0.007%
29	5.040	1228	1244	1267	rBV2	602134	1576492	100.00%	12.784%
30	5.551	1399	1403	1405	rBV5	2548	1930	0.12%	0.016%
31	5.613	1411	1422	1449	rBV	519288	1046736	66.40%	8.488%
32	6.066	1551	1563	1583	rBV	367829	738116	46.82%	5.986%
33	6.876	1812	1815	1816	rBV2	1428	902	0.06%	0.007%
34	6.982	1835	1848	1873	rBV	172402	330590	20.97%	2.681%
35	7.143	1896	1898	1902	rBV5	1452	1050	0.07%	0.009%
36	7.217	1917	1921	1923	rBV5	1649	1276	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028788.D
 Acq On : 31 Oct 2022 18:18
 Operator : SY/MD
 Sample : N5354-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBMP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	7.310	1939	1950	1971	rBV	675256	1176971	74.66%	9.544%
38	7.616	2036	2045	2063	rBV2	110222	201092	12.76%	1.631%
39	8.085	2182	2191	2221	rBV	427837	842195	53.42%	6.830%
40	8.616	2354	2356	2357	rBV2	777	245	0.02%	0.002%
41	8.648	2363	2366	2368	rBV4	1664	798	0.05%	0.006%
42	8.699	2379	2382	2383	rBV2	1625	806	0.05%	0.007%
43	8.744	2394	2396	2401	rVB6	1815	1092	0.07%	0.009%
44	8.847	2416	2428	2449	rBV	753743	1244460	78.94%	10.092%
45	9.143	2513	2520	2525	rBV10	3181	4765	0.30%	0.039%
46	9.223	2543	2545	2546	rBV2	2215	879	0.06%	0.007%
47	9.272	2557	2560	2563	rBV6	1351	903	0.06%	0.007%
48	9.304	2568	2570	2572	rBV3	1631	759	0.05%	0.006%
49	9.342	2578	2582	2586	rBV5	1769	1495	0.09%	0.012%
50	9.484	2621	2626	2629	rVB4	2565	2130	0.14%	0.017%
51	9.545	2635	2645	2649	rBV4	6408	12014	0.76%	0.097%
52	9.648	2675	2677	2680	rBV4	1392	903	0.06%	0.007%
53	9.722	2693	2700	2702	rBV7	2214	2356	0.15%	0.019%
54	9.908	2755	2758	2761	rBV4	2013	1535	0.10%	0.012%
55	9.992	2780	2784	2786	rBV5	2040	1659	0.11%	0.013%
56	10.082	2807	2812	2814	rBV7	2116	1552	0.10%	0.013%
57	10.207	2839	2851	2874	rBV	466773	746737	47.37%	6.056%
58	10.696	3001	3003	3010	rVB7	1414	962	0.06%	0.008%
59	10.744	3017	3018	3021	rVB3	1217	406	0.03%	0.003%
60	10.763	3022	3024	3025	rBV2	1740	558	0.04%	0.005%
61	11.037	3104	3109	3110	rBV4	1908	1261	0.08%	0.010%
62	11.059	3114	3116	3117	rVV2	759	204	0.01%	0.002%
63	11.159	3145	3147	3148	rBV2	2183	1002	0.06%	0.008%
64	11.239	3162	3172	3193	rBV	672615	1075093	68.20%	8.718%
65	11.616	3278	3289	3314	rVB	608041	981195	62.24%	7.957%
66	11.870	3362	3368	3372	rBV8	2457	2874	0.18%	0.023%
67	12.021	3414	3415	3417	rBV2	1526	636	0.04%	0.005%
68	12.079	3428	3433	3436	rBV7	1330	1400	0.09%	0.011%
69	12.156	3455	3457	3458	rBV2	1070	465	0.03%	0.004%
70	12.207	3470	3473	3475	rBV3	2145	1324	0.08%	0.011%
71	12.516	3565	3569	3570	rBV4	1432	972	0.06%	0.008%
72	12.606	3594	3597	3600	rBV5	1666	1209	0.08%	0.010%
73	12.638	3604	3607	3609	rBV3	1641	1237	0.08%	0.010%
74	12.857	3669	3675	3676	rBV8	1600	1232	0.08%	0.010%
75	13.136	3761	3762	3765	rBV3	1387	598	0.04%	0.005%
76	13.403	3841	3845	3846	rBV4	1377	1034	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028788.D
Acq On : 31 Oct 2022 18:18
Operator : SY/MD
Sample : N5354-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBMP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M

Title : VOC Analysis

77	13.725	3938	3945	3947	rBV7	1536	1847	0.12%	0.015%
78	13.799	3964	3968	3970	rBV5	1832	1631	0.10%	0.013%
79	13.844	3980	3982	3988	rBV6	1981	1636	0.10%	0.013%
80	13.873	3989	3991	3997	rVV6	1943	1441	0.09%	0.012%
81	13.931	4006	4009	4014	rVB7	1025	868	0.06%	0.007%
82	13.956	4014	4017	4019	rBV4	2258	1239	0.08%	0.010%




Sum of corrected areas: 12331539

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028788.D
Acq On : 31 Oct 2022 18:18
Operator : SY/MD
Sample : N5354-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBMP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

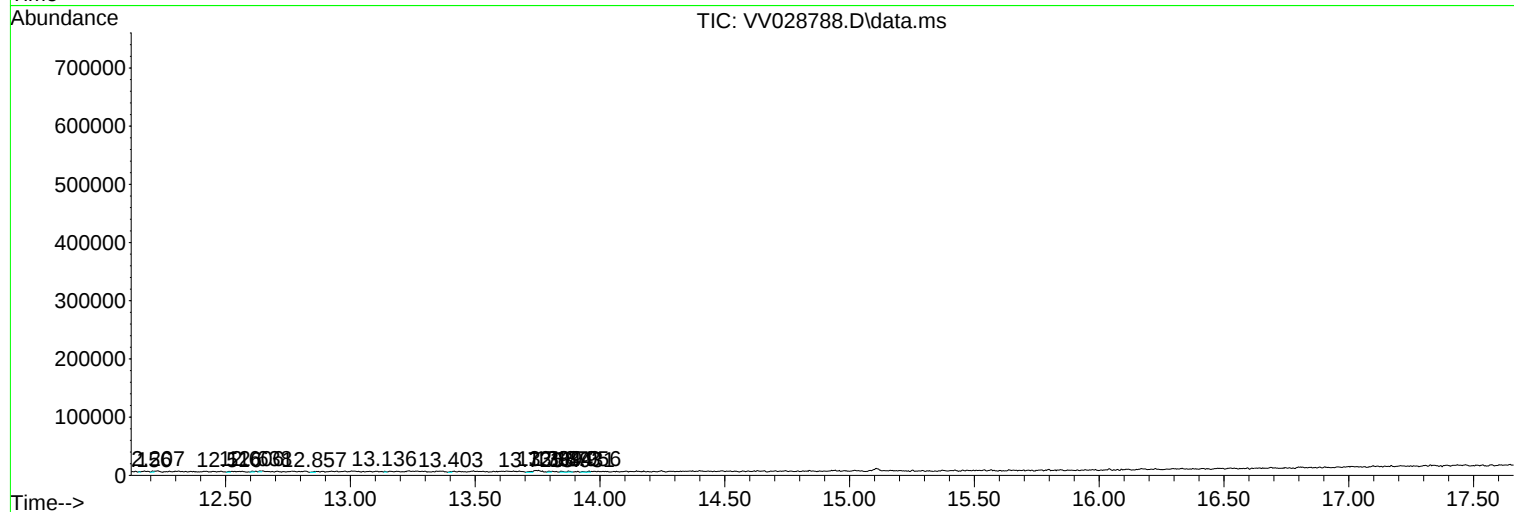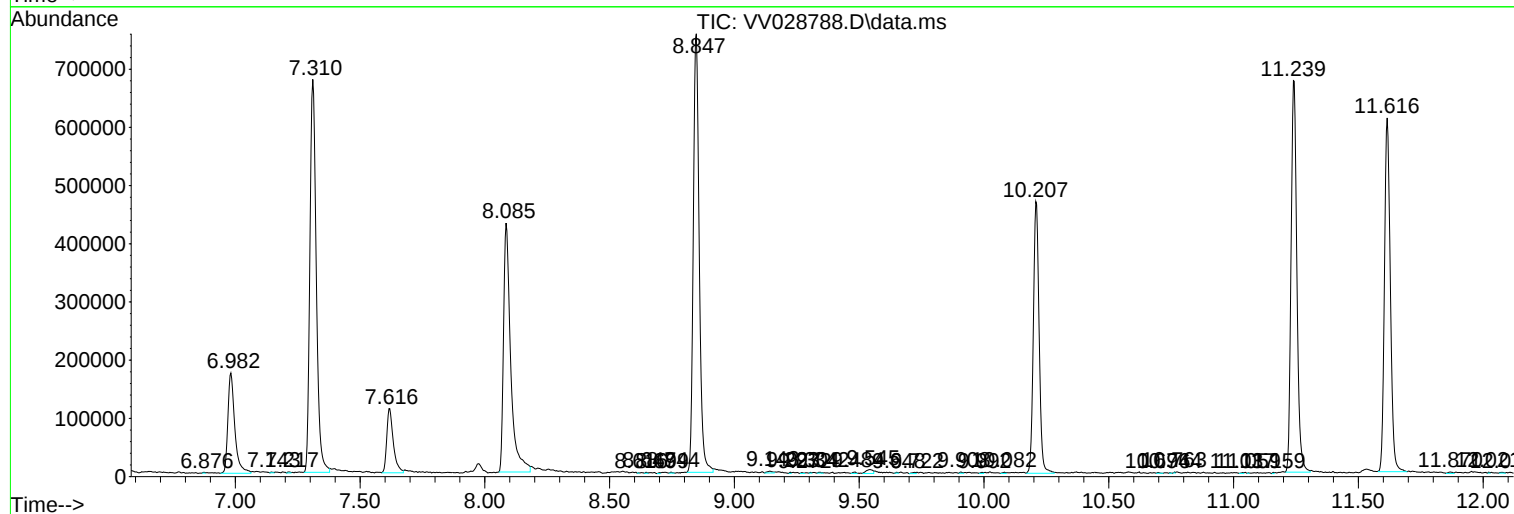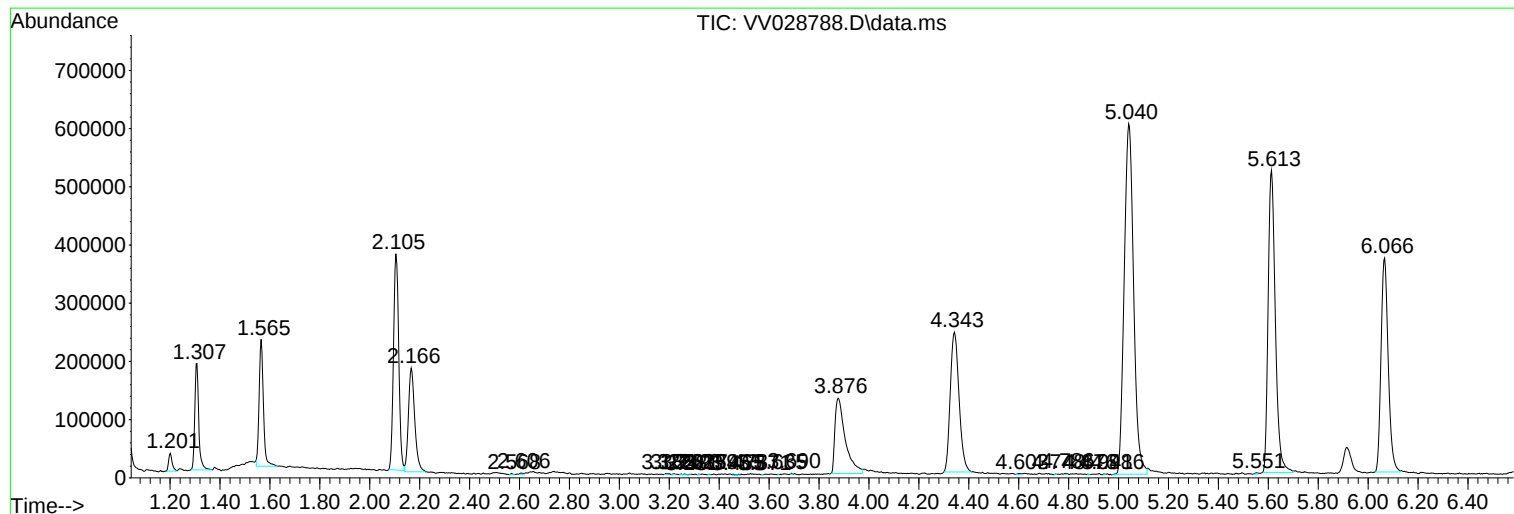

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028788.D
Acq On : 31 Oct 2022 18:18
Operator : SY/MD
Sample : N5354-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBMP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028788.D
Acq On : 31 Oct 2022 18:18
Operator : SY/MD
Sample : N5354-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBMP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc