

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028790.D
 Acq On : 31 Oct 2022 19:07
 Operator : SY/MD
 Sample : N5354-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBMP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028790.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	102	rVB	183785	205499	13.10%	1.561%
2	1.564	157	163	178	rVB	216633	248663	15.85%	1.888%
3	2.105	323	331	344	rVB	368998	523547	33.36%	3.976%
4	2.886	572	574	575	rBV2	1233	571	0.04%	0.004%
5	3.018	611	615	618	rBV5	1695	1813	0.12%	0.014%
6	3.082	633	635	636	rBV2	1431	526	0.03%	0.004%
7	3.124	647	648	651	rBV3	1249	435	0.03%	0.003%
8	3.166	659	661	662	rBV2	1365	451	0.03%	0.003%
9	3.359	719	721	722	rVB2	1265	394	0.03%	0.003%
10	3.407	734	736	739	rBV3	1288	631	0.04%	0.005%
11	3.439	742	746	748	rVV6	1283	935	0.06%	0.007%
12	3.478	756	758	763	rVB5	1710	1001	0.06%	0.008%
13	3.500	763	765	766	rBV2	750	196	0.01%	0.001%
14	3.519	767	771	772	rBV4	1478	1023	0.07%	0.008%
15	3.548	778	780	783	rBV4	1496	891	0.06%	0.007%
16	3.629	803	805	807	rBV3	1045	496	0.03%	0.004%
17	3.648	807	811	814	rVV7	1417	1239	0.08%	0.009%
18	3.693	821	825	826	rBV3	1505	1170	0.07%	0.009%
19	3.773	847	850	852	rBV4	1247	712	0.05%	0.005%
20	3.793	852	856	860	rVV6	1674	1553	0.10%	0.012%
21	3.896	873	888	918	rBV3	161685	623843	39.76%	4.738%
22	4.342	1011	1027	1047	rBV	241218	601688	38.34%	4.569%
23	4.757	1154	1156	1159	rBV4	1168	718	0.05%	0.005%
24	4.802	1168	1170	1172	rVB3	971	324	0.02%	0.002%
25	4.838	1179	1181	1182	rBV2	1091	468	0.03%	0.004%
26	5.040	1228	1244	1270	rBV2	600744	1569179	100.00%	11.917%
27	5.465	1373	1376	1377	rBV3	1392	751	0.05%	0.006%
28	5.613	1411	1422	1451	rBV	529532	1063886	67.80%	8.079%
29	5.908	1503	1514	1538	rBV	471386	929202	59.22%	7.057%
30	6.066	1552	1563	1590	rVB	364300	746152	47.55%	5.666%
31	6.645	1741	1743	1745	rBV3	2355	960	0.06%	0.007%
32	6.982	1839	1848	1867	rBV	167398	298879	19.05%	2.270%
33	7.310	1939	1950	1986	rBV	661822	1183747	75.44%	8.990%
34	7.619	2036	2046	2064	rBV	108481	199024	12.68%	1.511%
35	7.812	2103	2106	2107	rBV2	1190	700	0.04%	0.005%
36	8.085	2182	2191	2217	rBV	395815	793615	50.58%	6.027%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028790.D
 Acq On : 31 Oct 2022 19:07
 Operator : SY/MD
 Sample : N5354-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBMP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	8.847	2417	2428	2454	rBV	769843	1269515	80.90%	9.641%
38	9.120	2511	2513	2515	rBV3	2387	1342	0.09%	0.010%
39	9.275	2559	2561	2562	rBV2	1395	602	0.04%	0.005%
40	9.352	2583	2585	2586	rBV2	670	155	0.01%	0.001%
41	9.545	2635	2645	2654	rBV3	11357	21194	1.35%	0.161%
42	9.722	2697	2700	2701	rBV3	867	634	0.04%	0.005%
43	9.796	2721	2723	2726	rBV4	1343	666	0.04%	0.005%
44	9.847	2737	2739	2743	rVB5	1577	987	0.06%	0.007%
45	9.870	2744	2746	2747	rBV2	1189	396	0.03%	0.003%
46	10.046	2797	2801	2802	rBV4	1535	940	0.06%	0.007%
47	10.156	2833	2835	2839	rVB5	1217	513	0.03%	0.004%
48	10.207	2839	2851	2871	rBV	459953	734594	46.81%	5.579%
49	10.461	2928	2930	2931	rBV2	1427	700	0.04%	0.005%
50	10.513	2944	2946	2948	rBV4	1394	537	0.03%	0.004%
51	10.622	2977	2980	2984	rBV6	2511	2491	0.16%	0.019%
52	10.699	3003	3004	3005	rBV	734	158	0.01%	0.001%
53	10.882	3059	3061	3062	rBV2	1859	800	0.05%	0.006%
54	11.030	3104	3107	3108	rBV2	1805	914	0.06%	0.007%
55	11.091	3124	3126	3128	rBV2	987	412	0.03%	0.003%
56	11.127	3135	3137	3141	rVB6	2053	1280	0.08%	0.010%
57	11.159	3141	3147	3152	rBV9	2487	3604	0.23%	0.027%
58	11.239	3162	3172	3192	rBV	693457	1101438	70.19%	8.365%
59	11.509	3254	3256	3258	rBV3	1588	997	0.06%	0.008%
60	11.558	3269	3271	3275	rVB5	2112	1071	0.07%	0.008%
61	11.616	3277	3289	3310	rBV	622716	985520	62.80%	7.484%
62	11.779	3338	3340	3345	rBV5	2573	1737	0.11%	0.013%
63	11.969	3394	3399	3403	rBV8	1676	2263	0.14%	0.017%
64	12.091	3434	3437	3441	rBV6	1695	1381	0.09%	0.010%
65	12.143	3452	3453	3455	rBV2	1207	425	0.03%	0.003%
66	12.162	3455	3459	3464	rBV7	1709	2328	0.15%	0.018%
67	12.381	3525	3527	3529	rBV3	1825	964	0.06%	0.007%
68	12.413	3535	3537	3539	rBV4	1454	766	0.05%	0.006%
69	12.493	3559	3562	3565	rBV5	1041	958	0.06%	0.007%
70	12.558	3581	3582	3584	rBV2	985	236	0.02%	0.002%
71	12.606	3595	3597	3598	rBV2	1055	385	0.02%	0.003%
72	12.725	3631	3634	3637	rBV5	838	560	0.04%	0.004%
73	12.773	3647	3649	3650	rBV2	1099	412	0.03%	0.003%
74	12.812	3659	3661	3665	rVB6	1341	571	0.04%	0.004%
75	12.844	3665	3671	3672	rBV5	1684	1338	0.09%	0.010%
76	12.998	3714	3719	3721	rBV6	2051	2166	0.14%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028790.D
 Acq On : 31 Oct 2022 19:07
 Operator : SY/MD
 Sample : N5354-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBMP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	13.059	3736	3738	3741	rVB4	1968	946	0.06%	0.007%
78	13.136	3758	3762	3764	rBV5	1560	1231	0.08%	0.009%
79	13.410	3843	3847	3851	rBV6	2468	2446	0.16%	0.019%
80	13.551	3889	3891	3892	rBV2	1204	453	0.03%	0.003%
81	13.689	3930	3934	3936	rBV5	1503	1062	0.07%	0.008%
82	13.731	3944	3947	3952	rBV7	1892	1716	0.11%	0.013%
83	13.876	3991	3992	3994	rBV2	1524	410	0.03%	0.003%
84	13.947	4011	4014	4015	rBV2	1568	835	0.05%	0.006%
85	14.104	4061	4063	4066	rBV3	2342	1483	0.09%	0.011%
86	14.204	4091	4094	4095	rBV3	1451	821	0.05%	0.006%
87	14.522	4191	4193	4197	rVB5	1777	1033	0.07%	0.008%
88	14.545	4197	4200	4202	rBV3	1529	944	0.06%	0.007%
89	14.783	4271	4274	4275	rBV4	1610	680	0.04%	0.005%
90	15.361	4452	4454	4457	rBV3	1582	1077	0.07%	0.008%




Sum of corrected areas: 13167969

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028790.D
Acq On : 31 Oct 2022 19:07
Operator : SY/MD
Sample : N5354-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBMP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

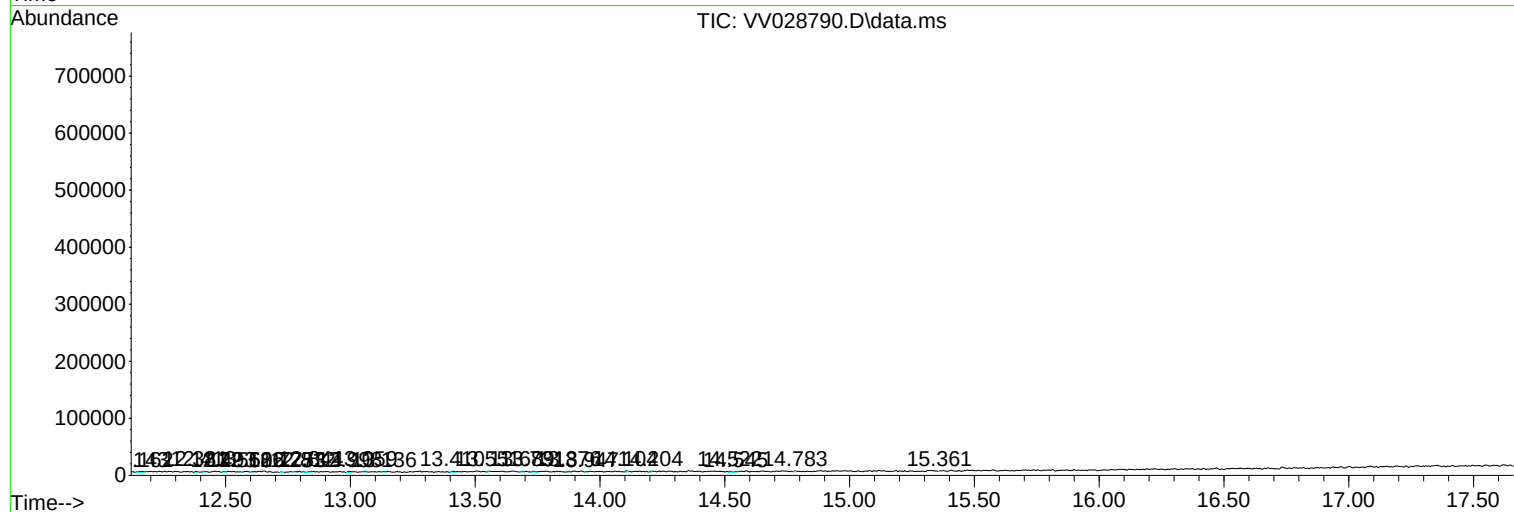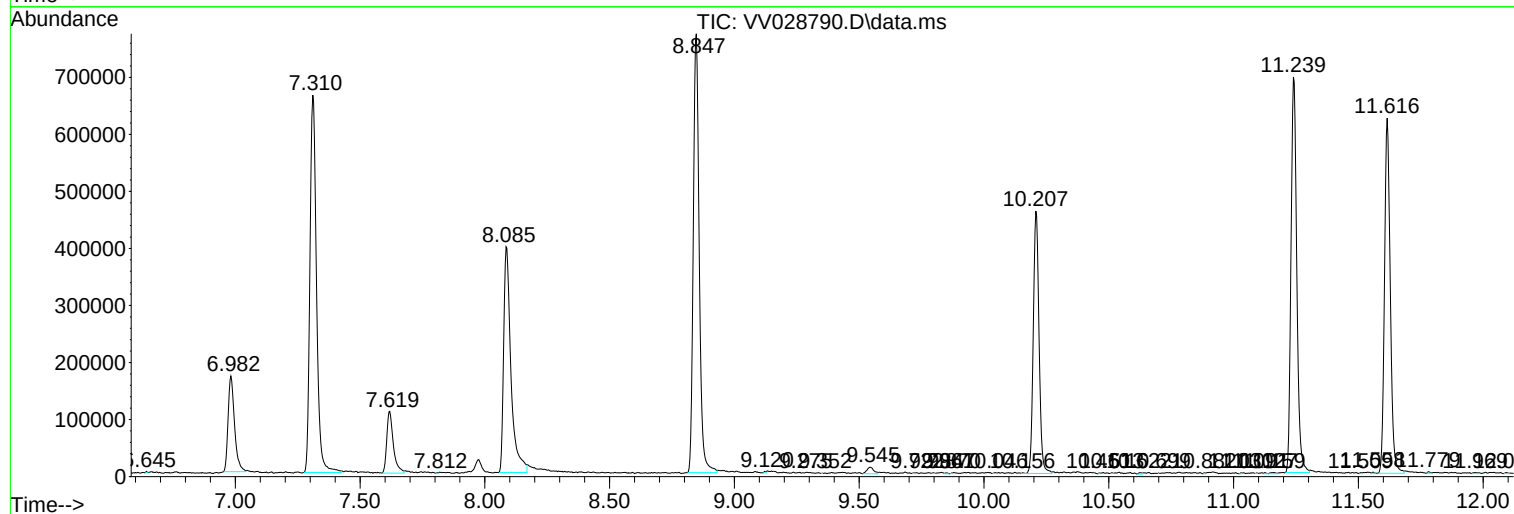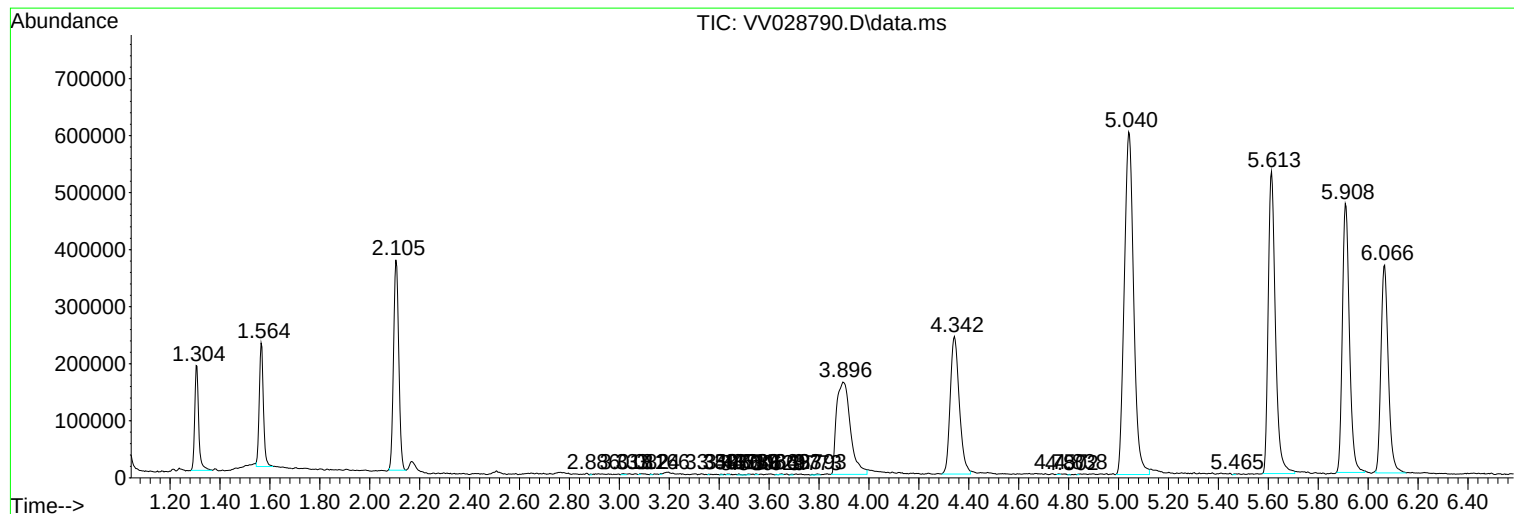

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028790.D
Acq On : 31 Oct 2022 19:07
Operator : SY/MD
Sample : N5354-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBMP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028790.D
Acq On : 31 Oct 2022 19:07
Operator : SY/MD
Sample : N5354-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBMP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc